

FIG.1

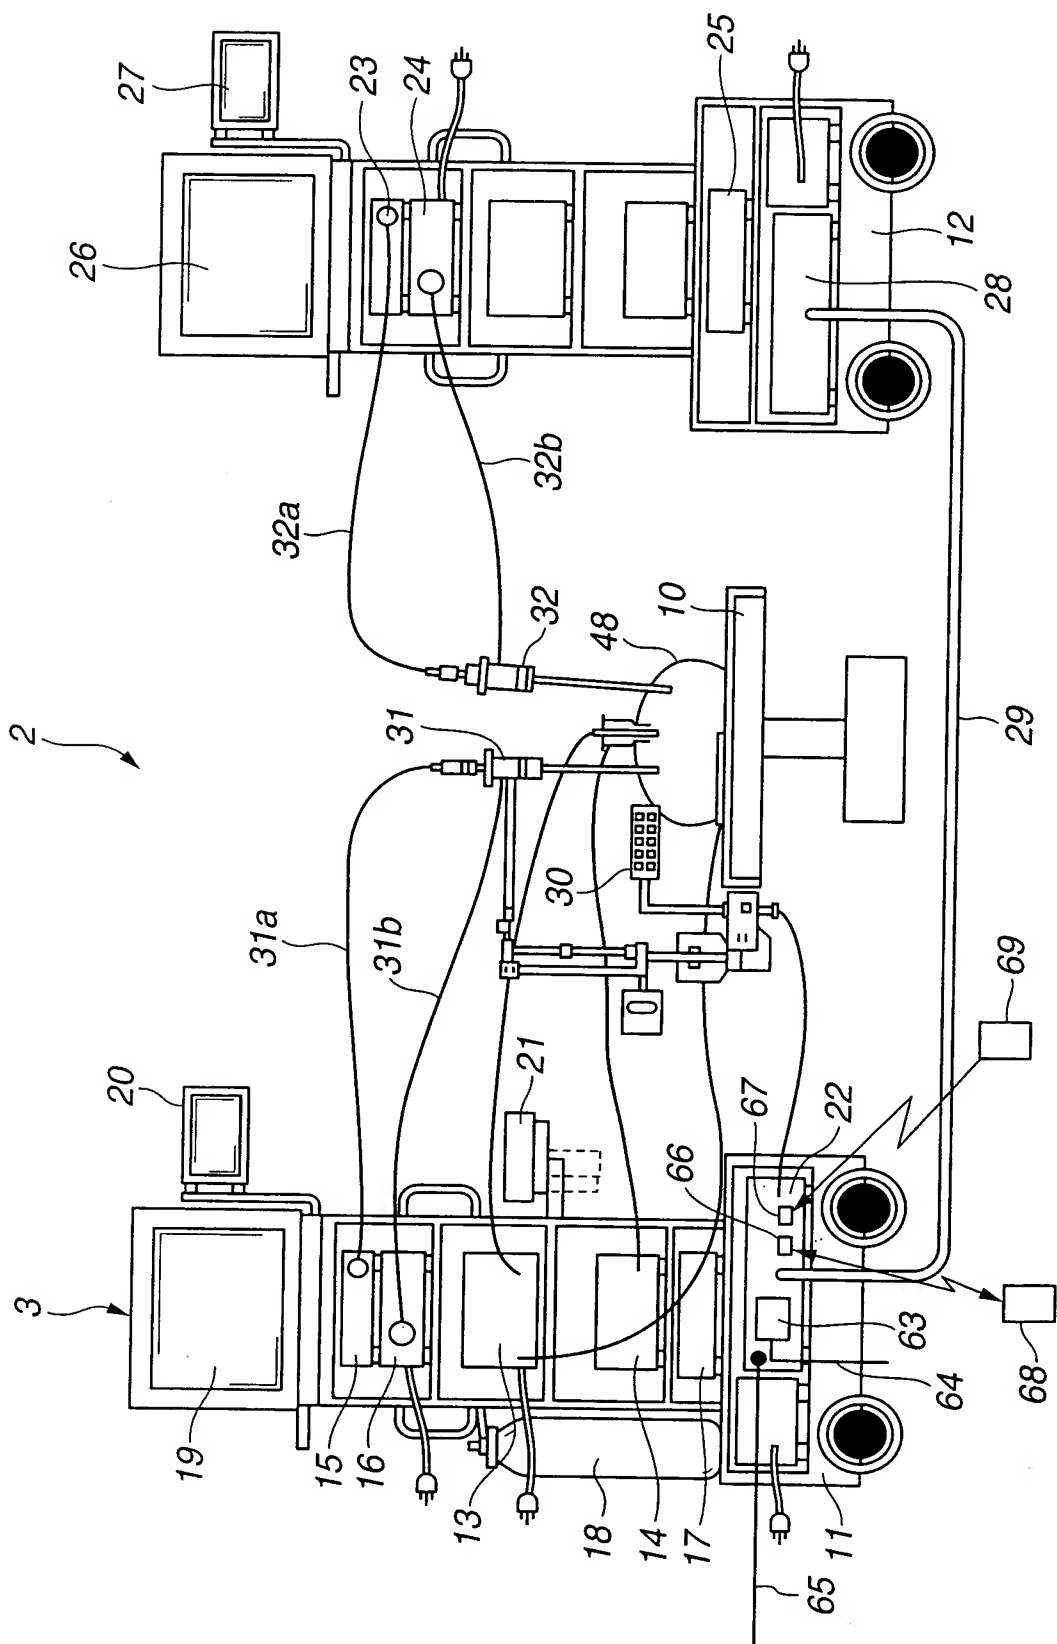


FIG.2

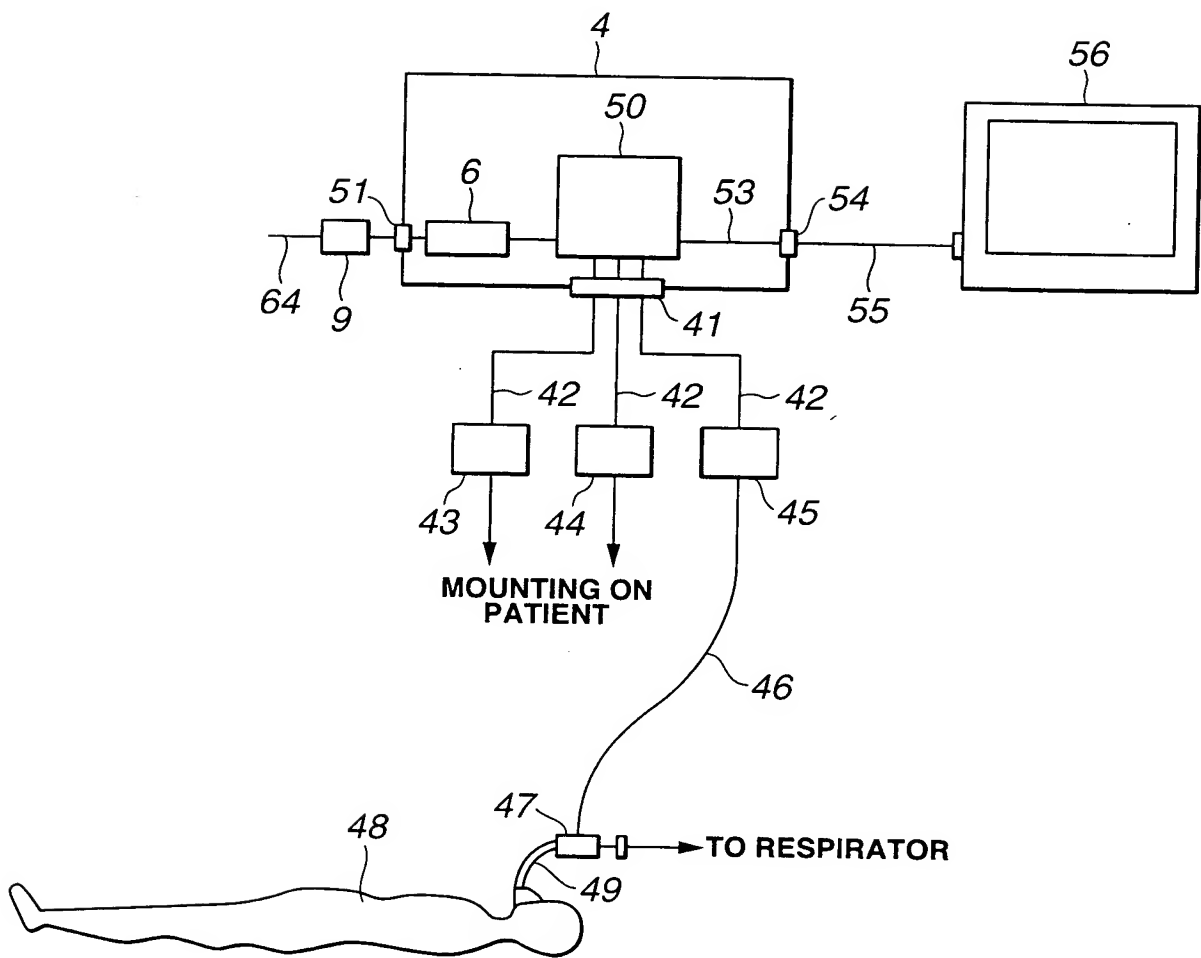


FIG.3

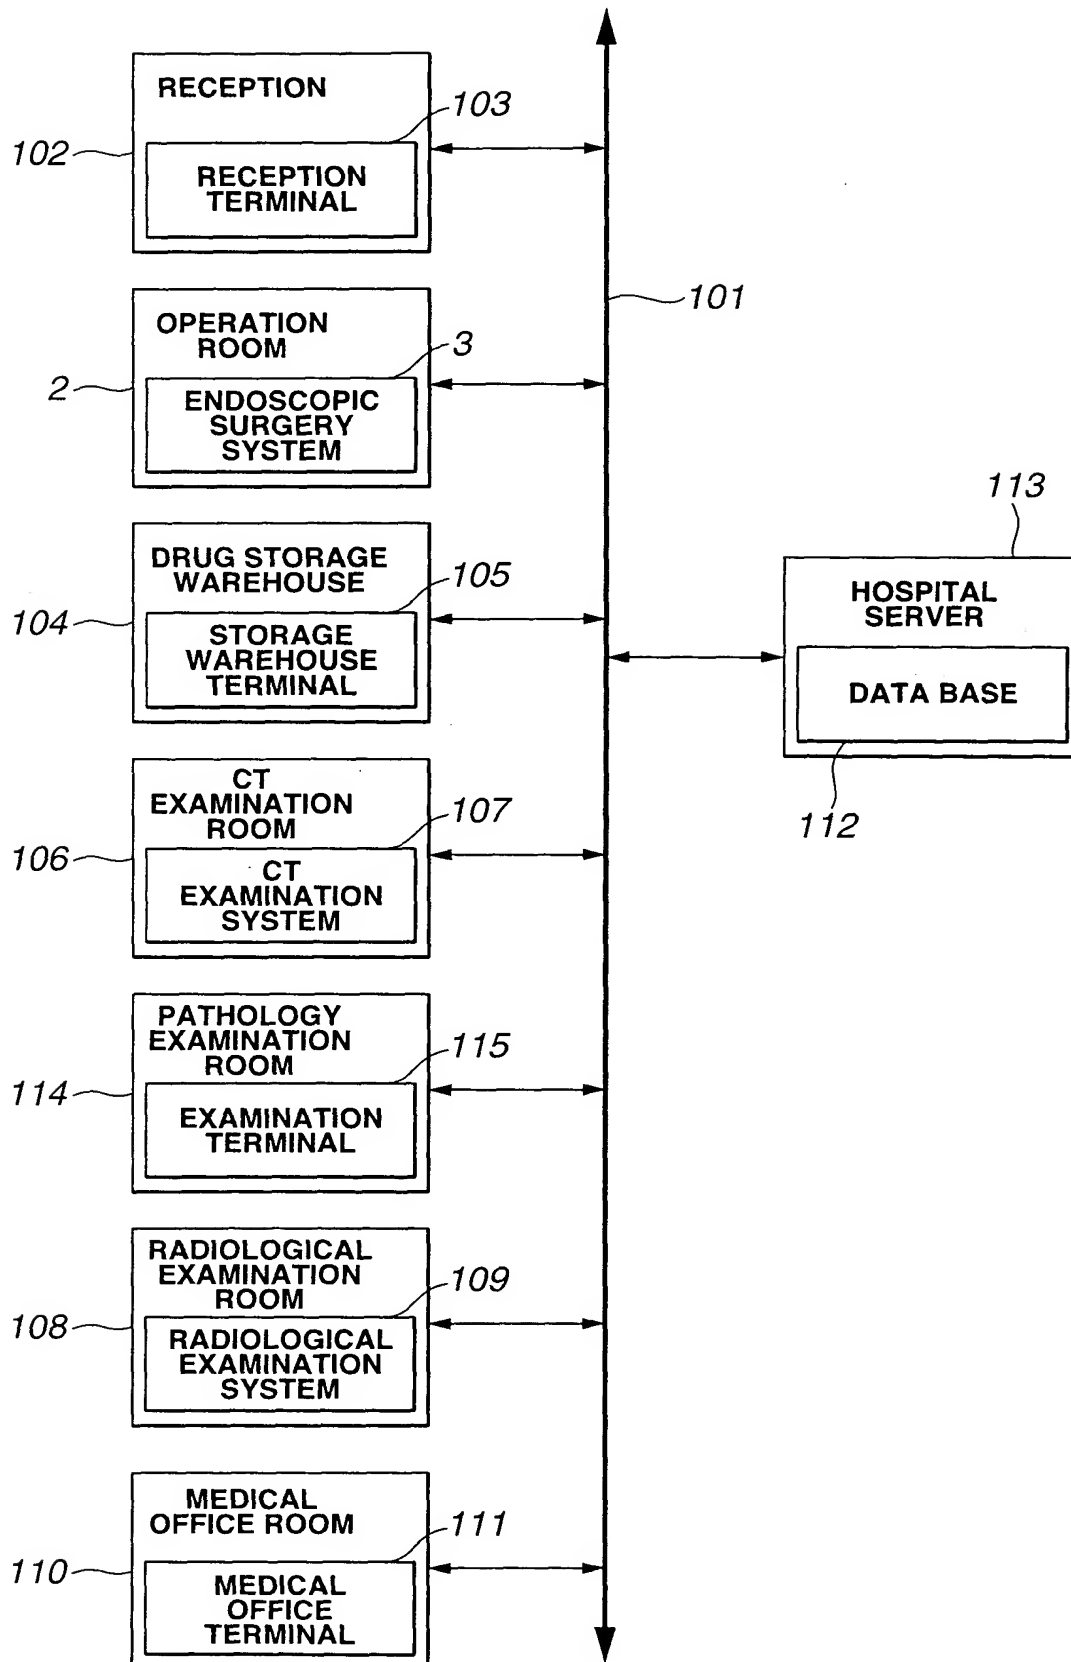


FIG.4

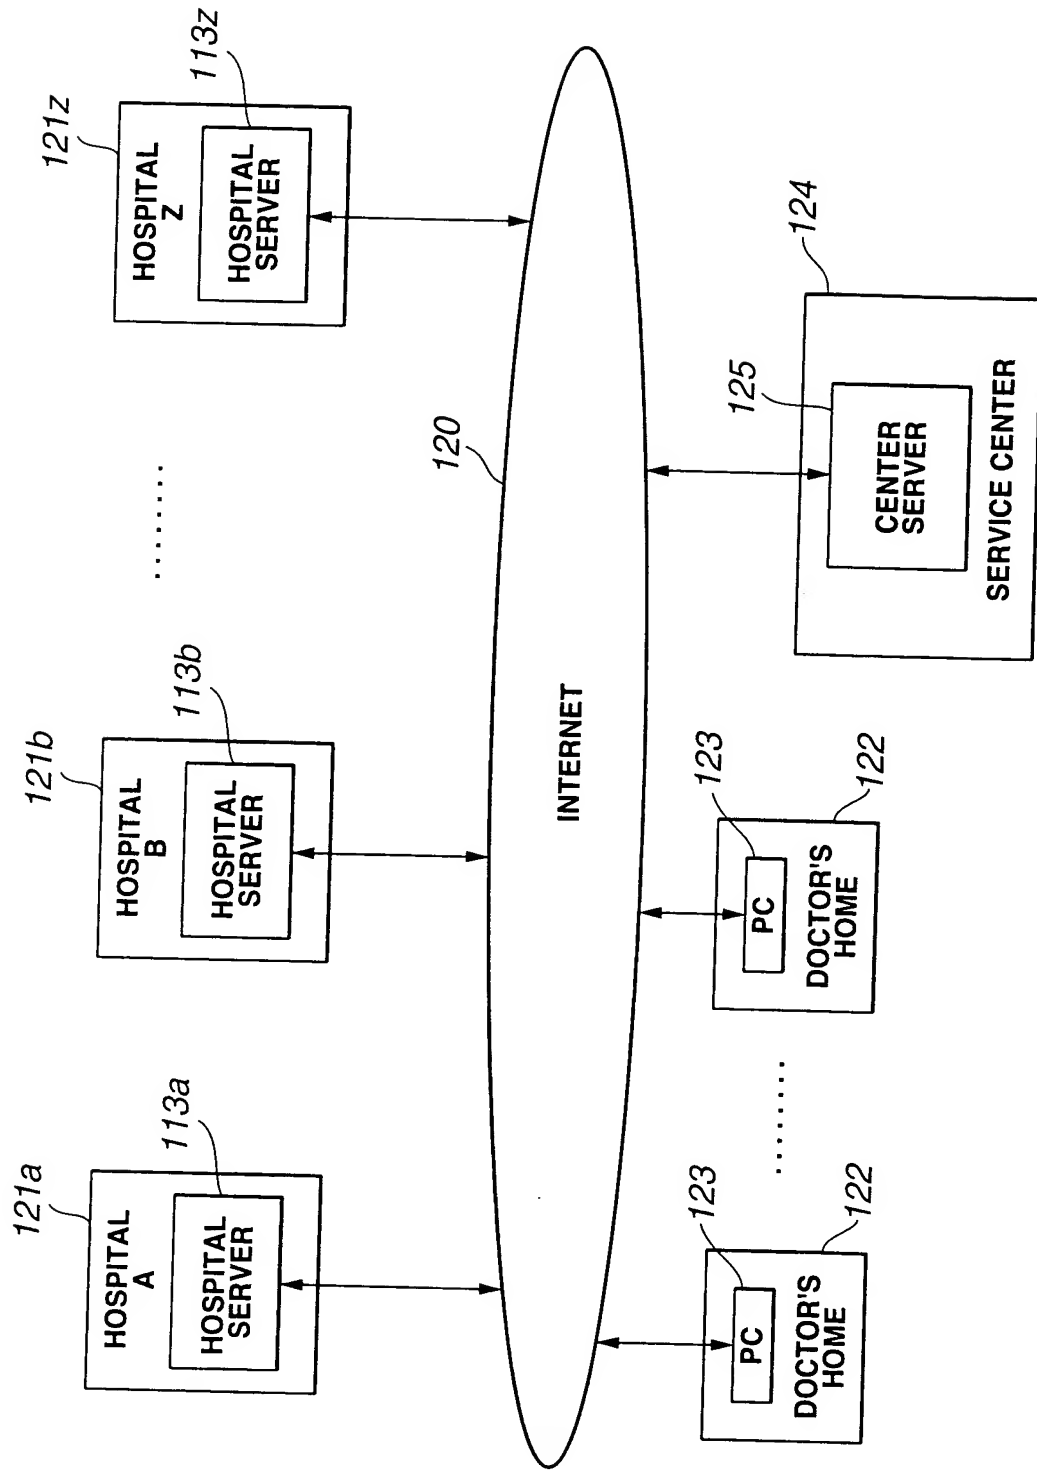


FIG.5

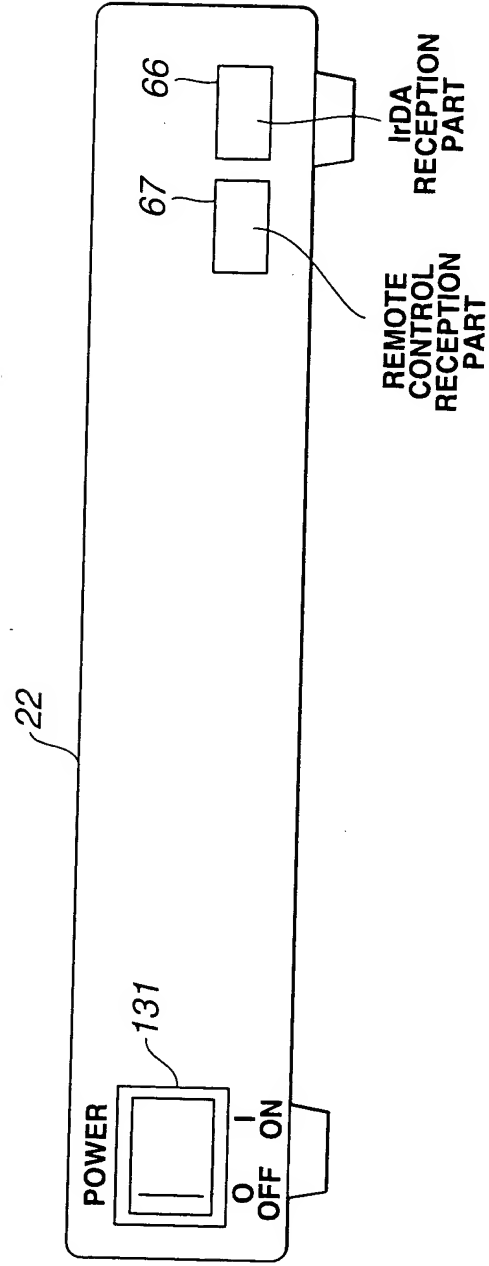


FIG.6

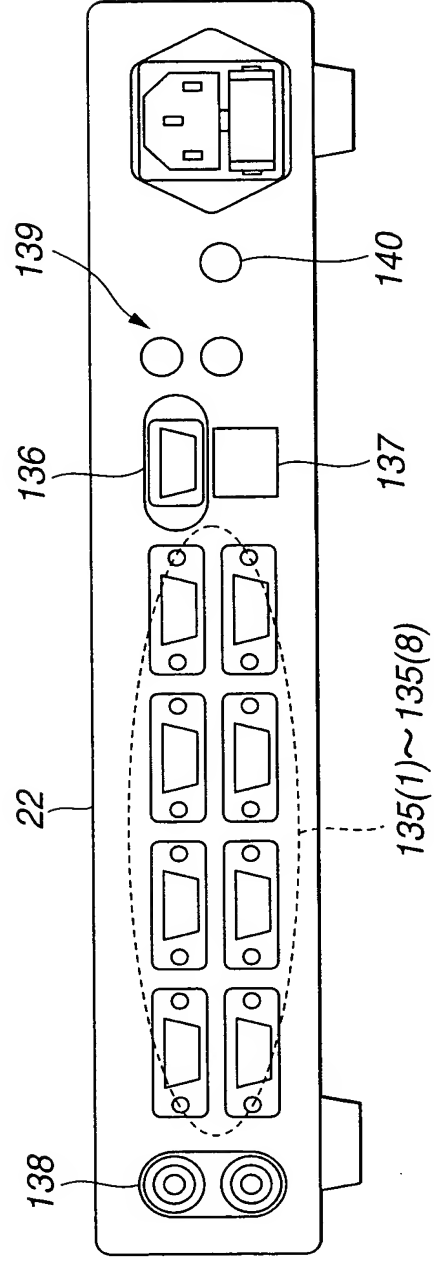


FIG. 7

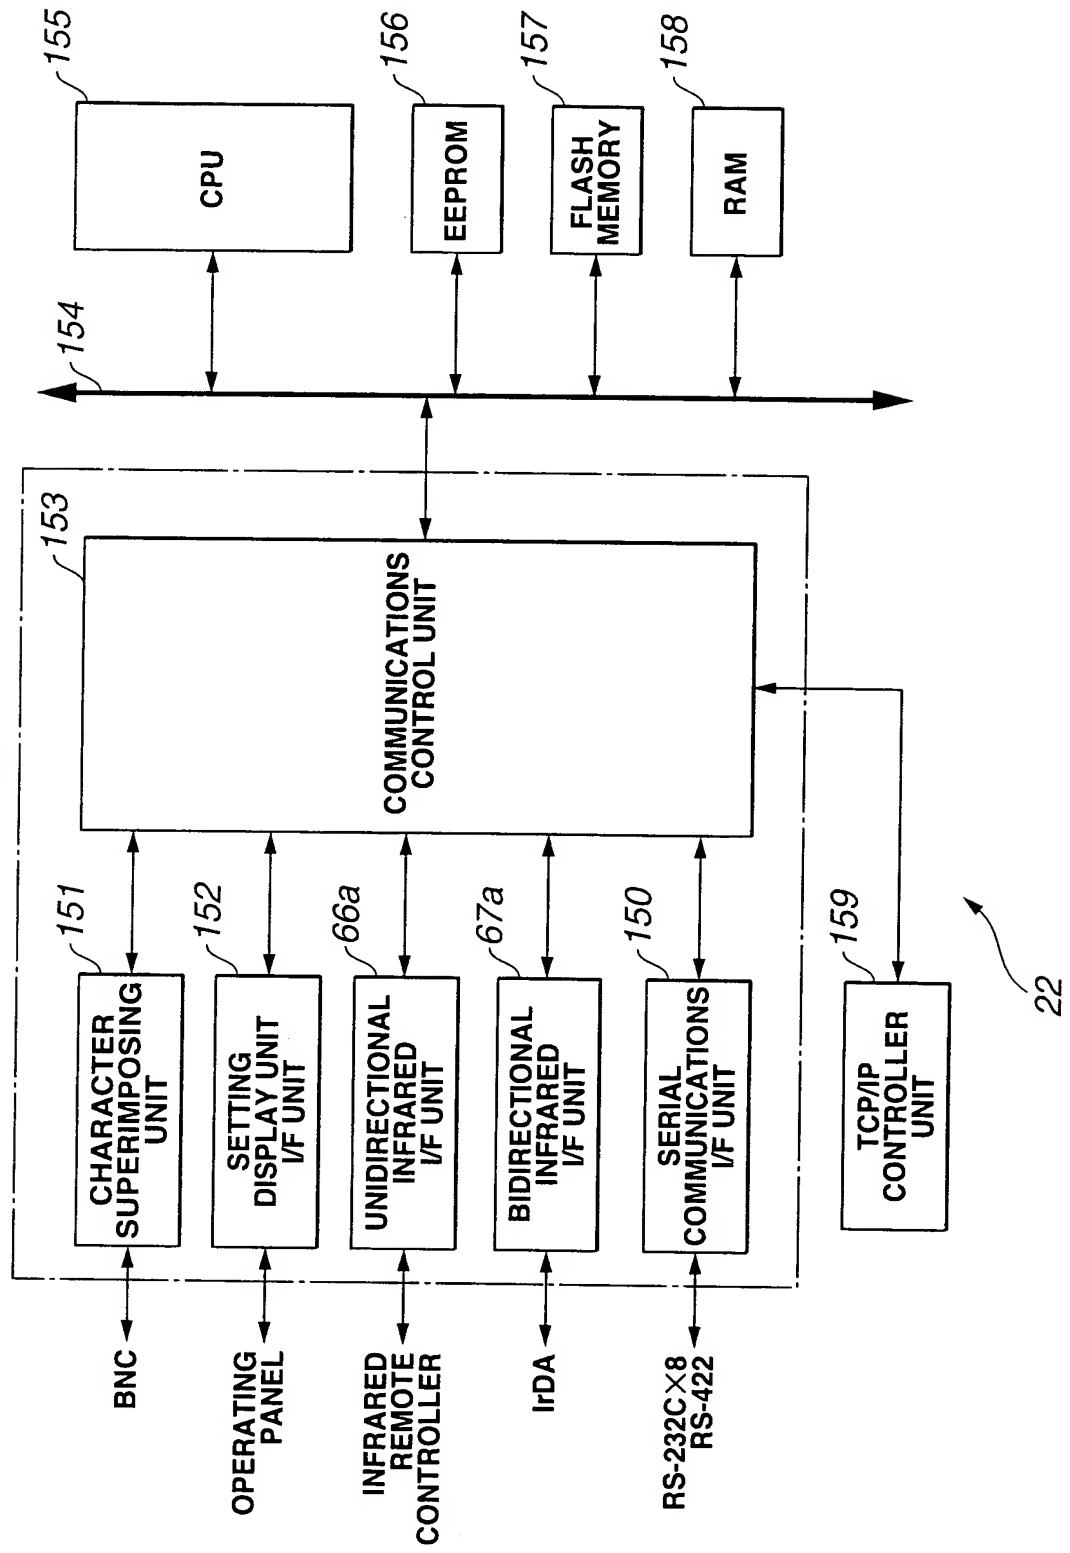


FIG. 8

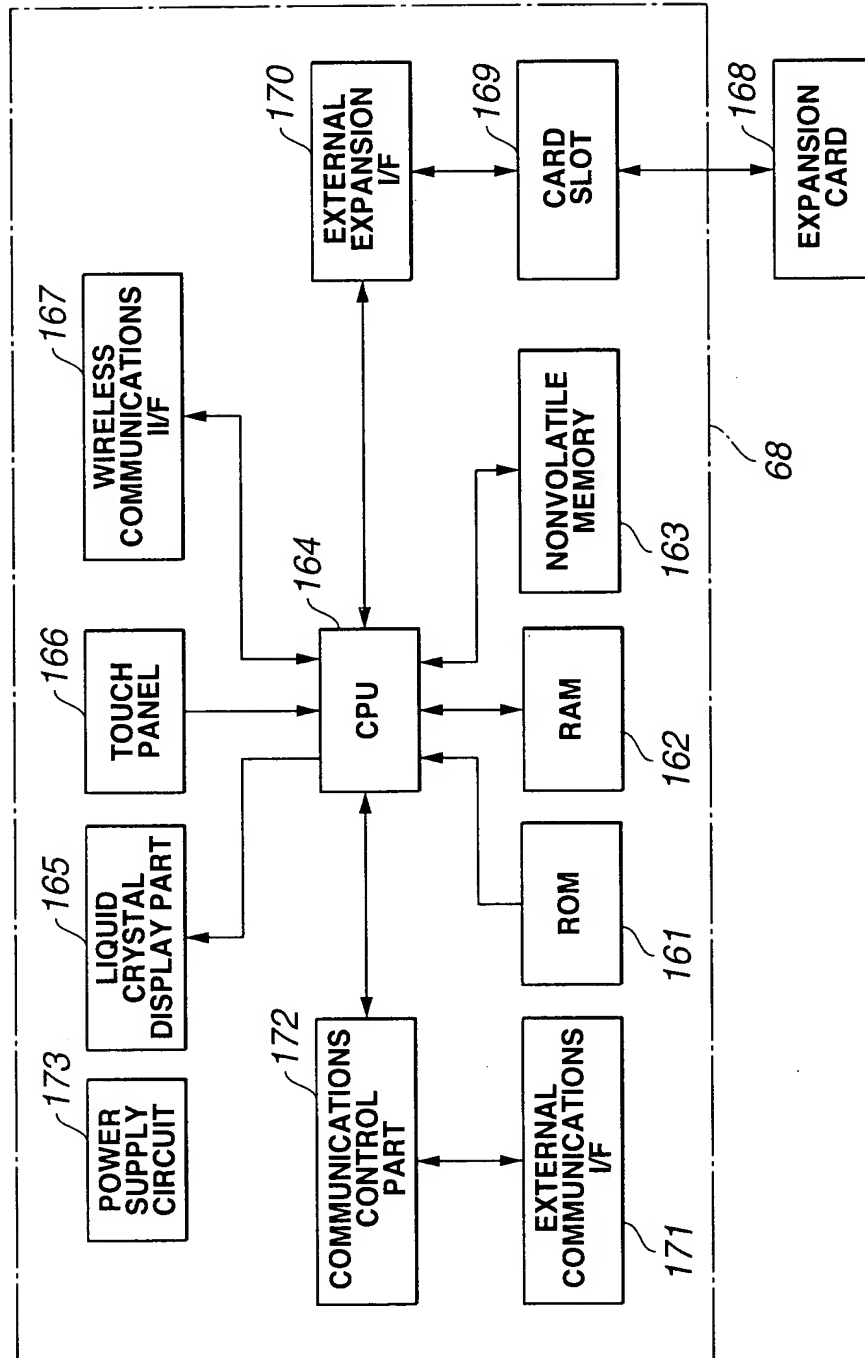


FIG.9

21

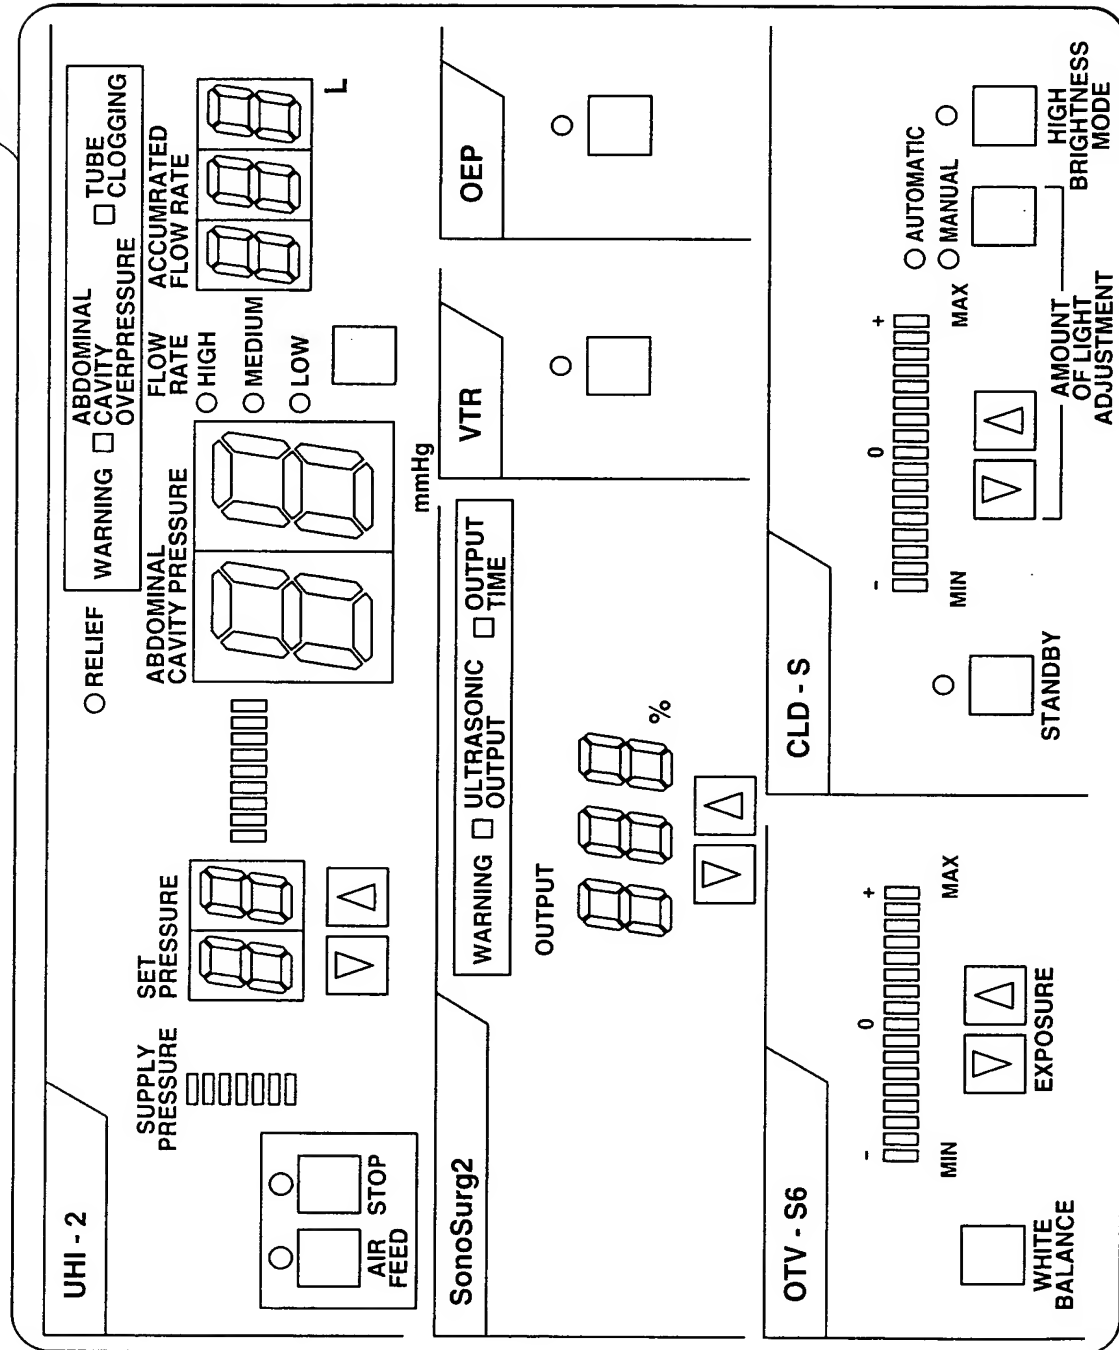


FIG.10

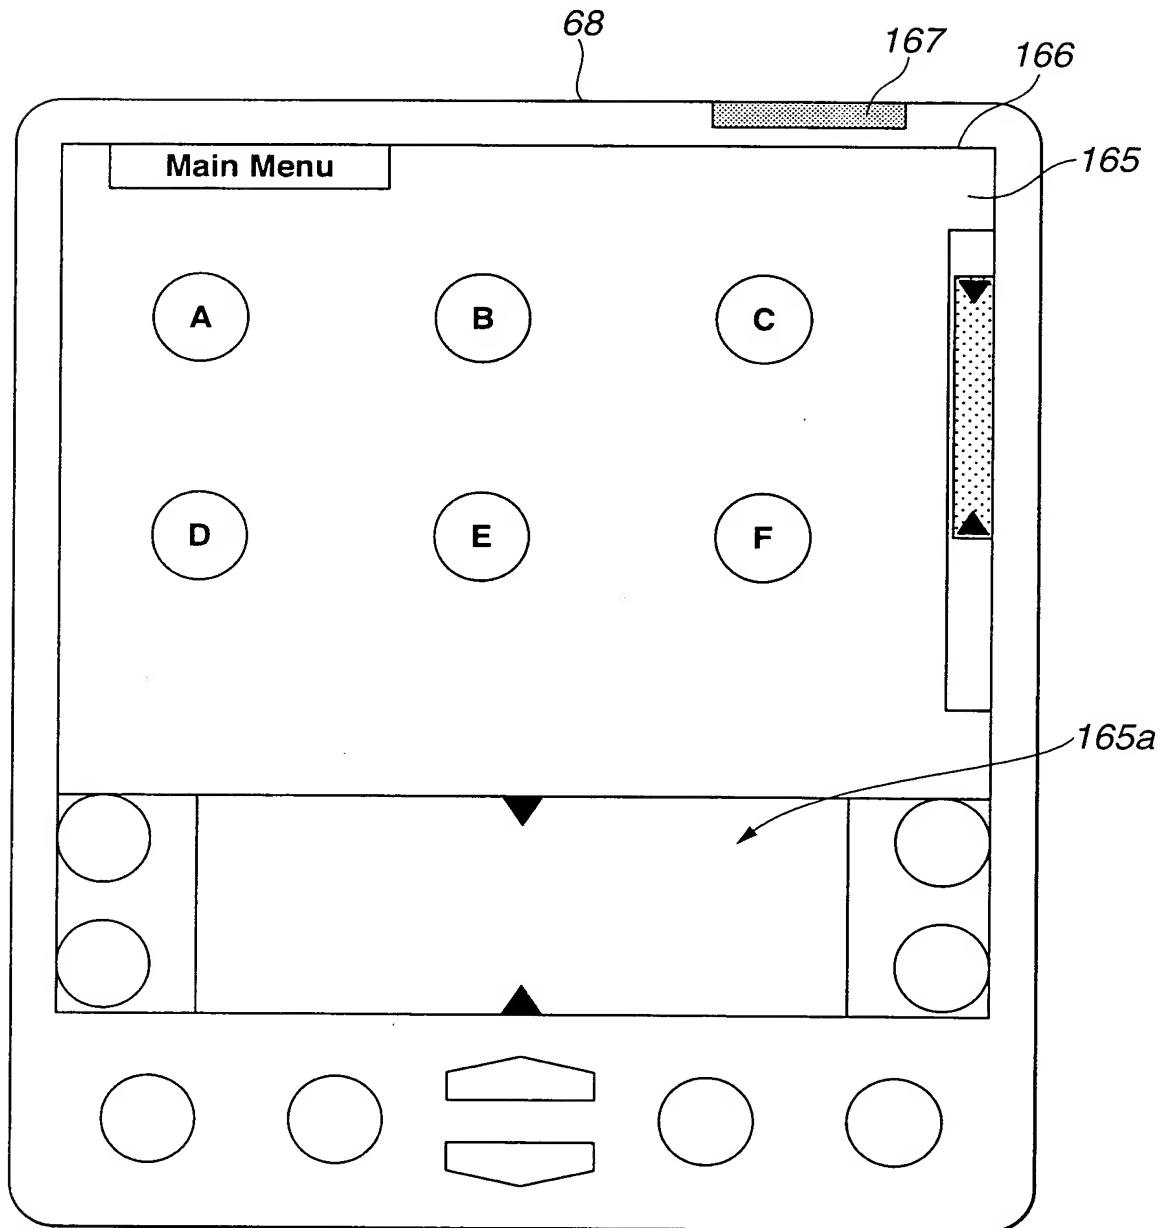


FIG.11

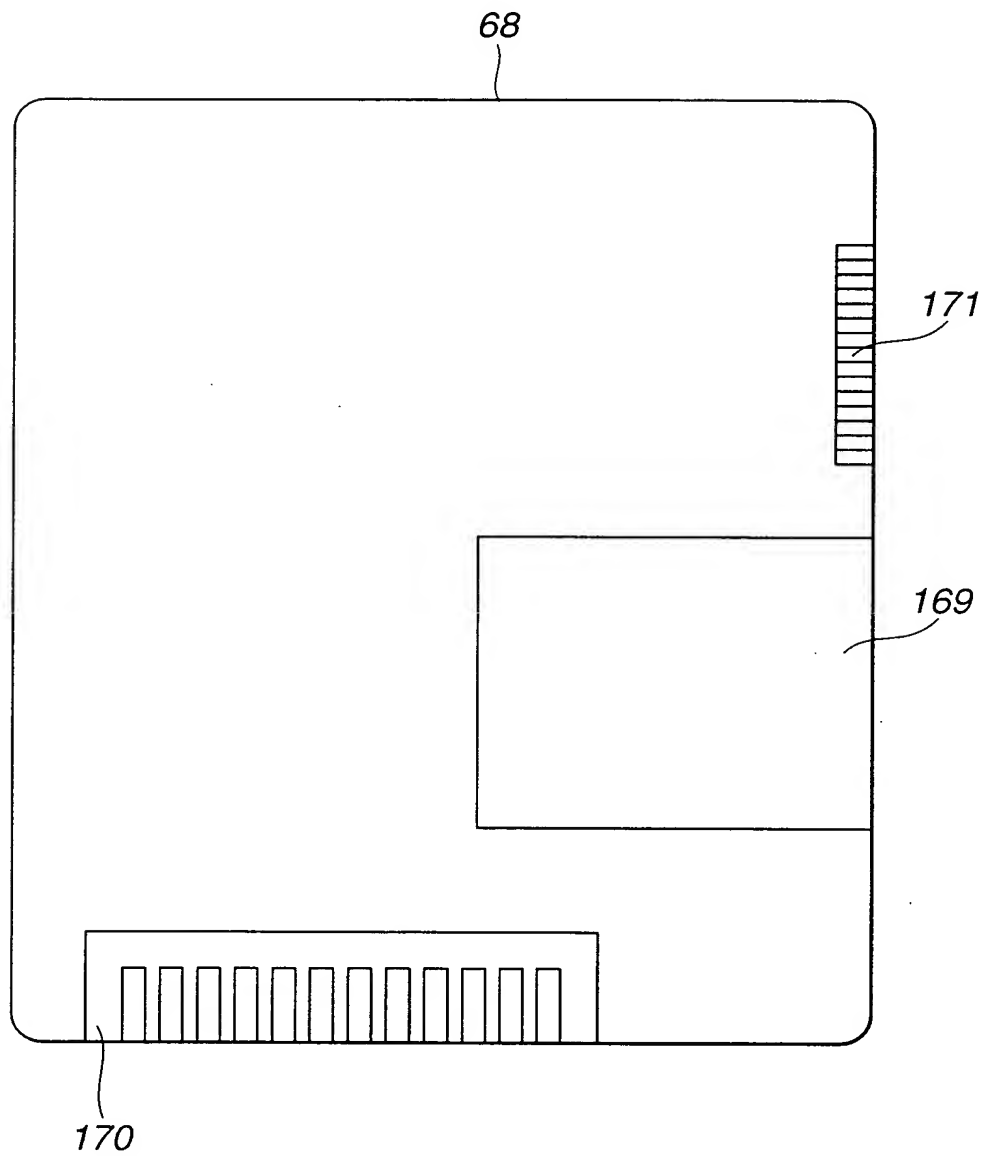


FIG.12

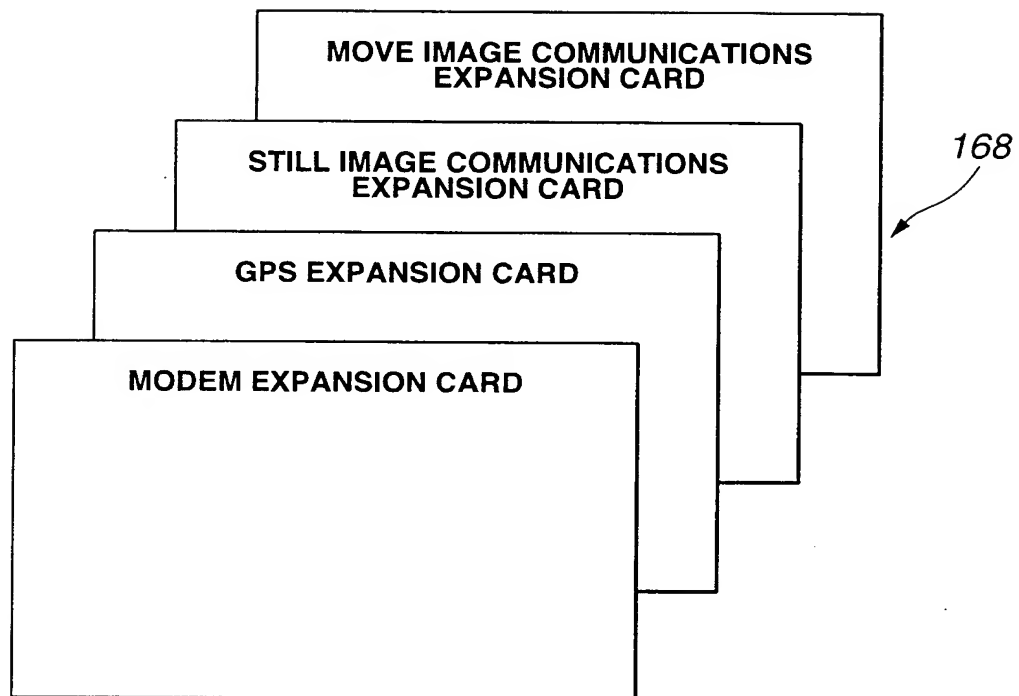


FIG.13

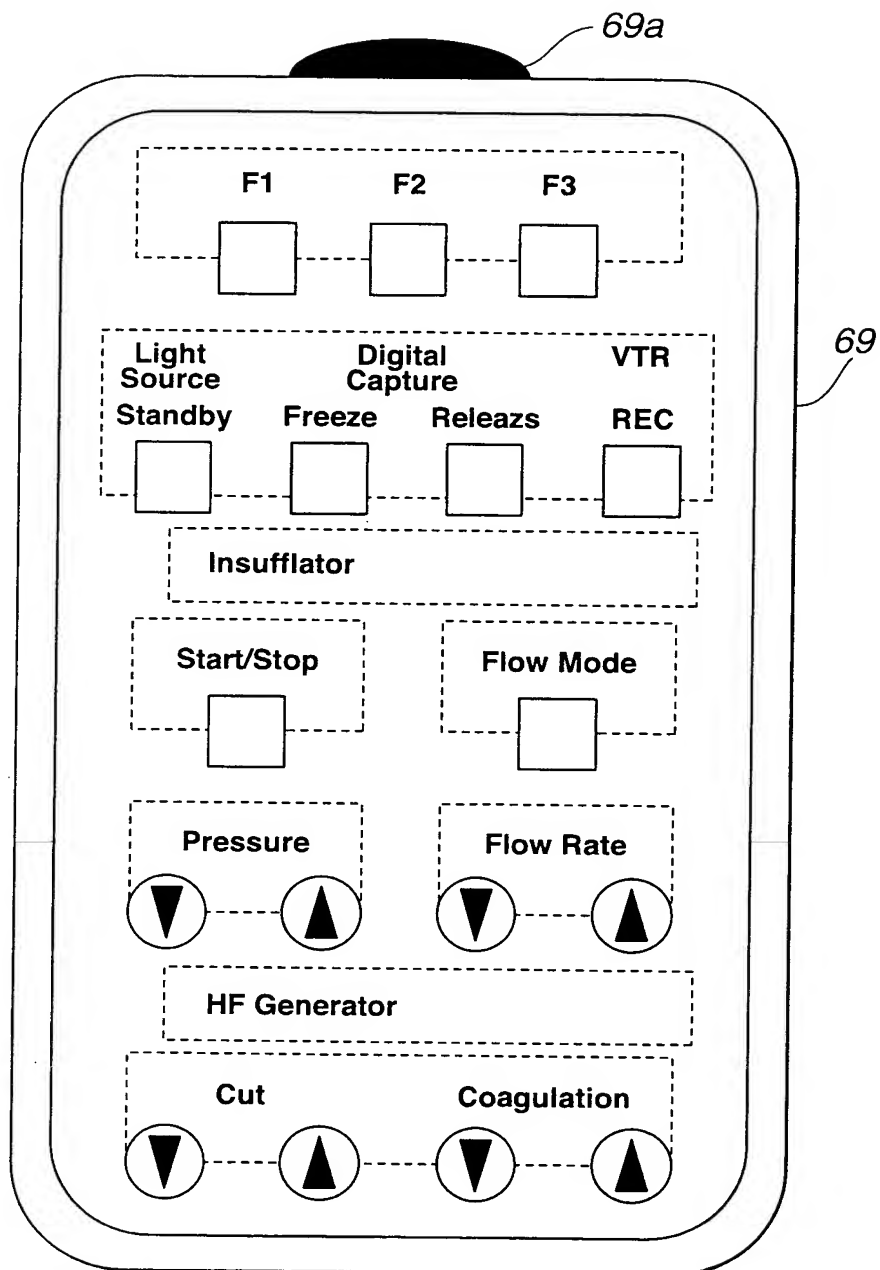


FIG.14

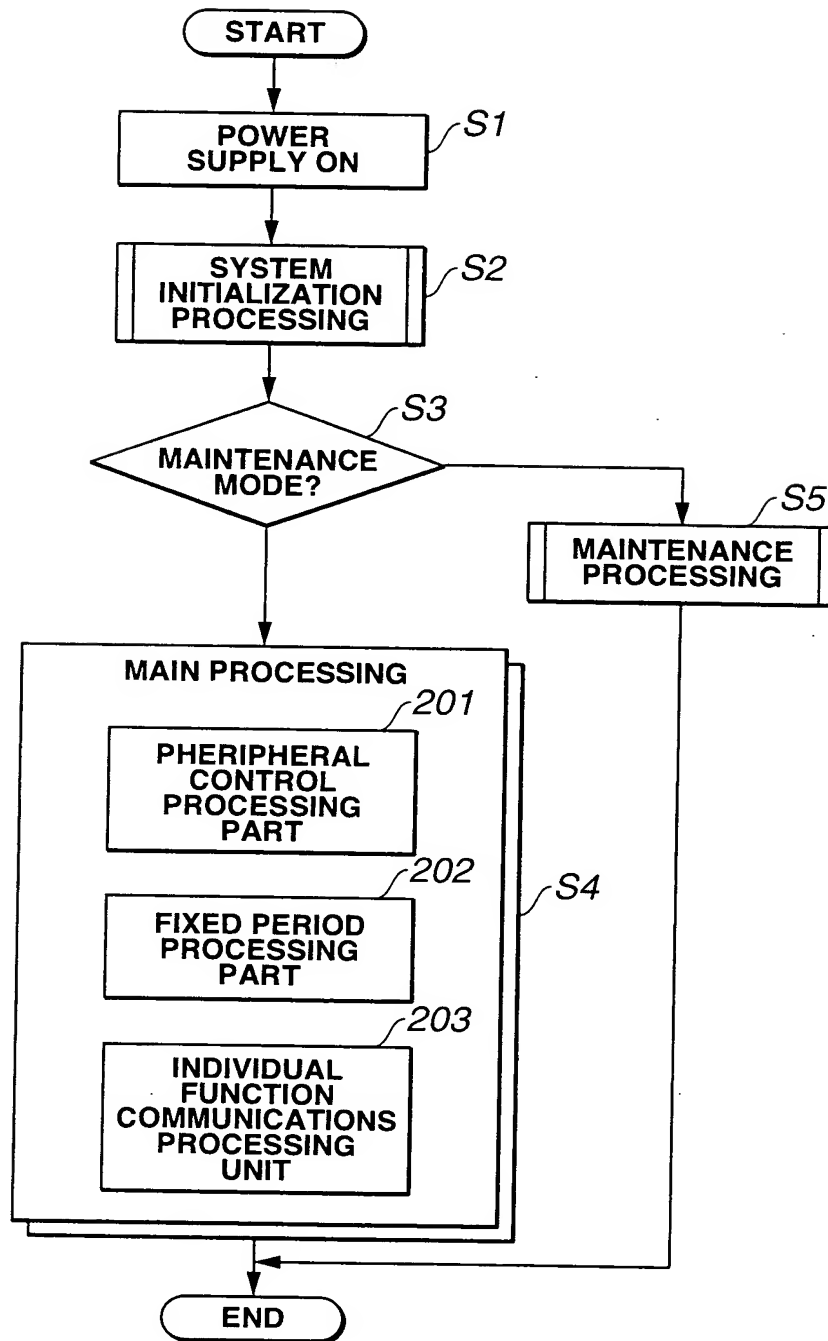


FIG.15

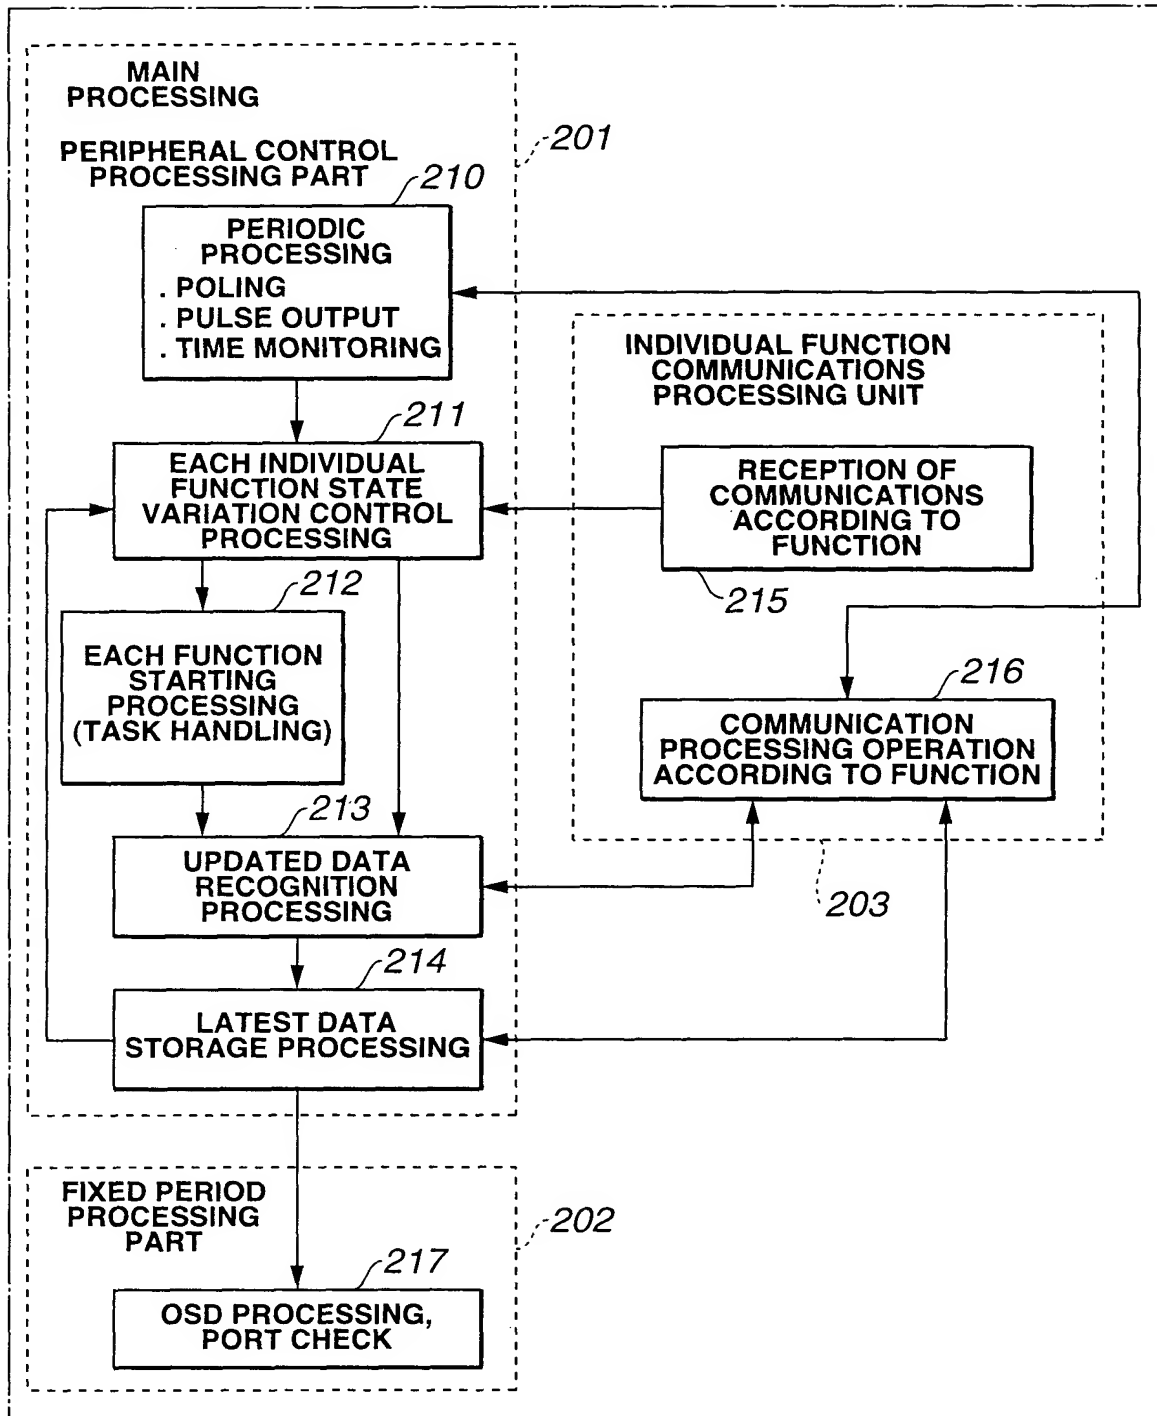


FIG.16

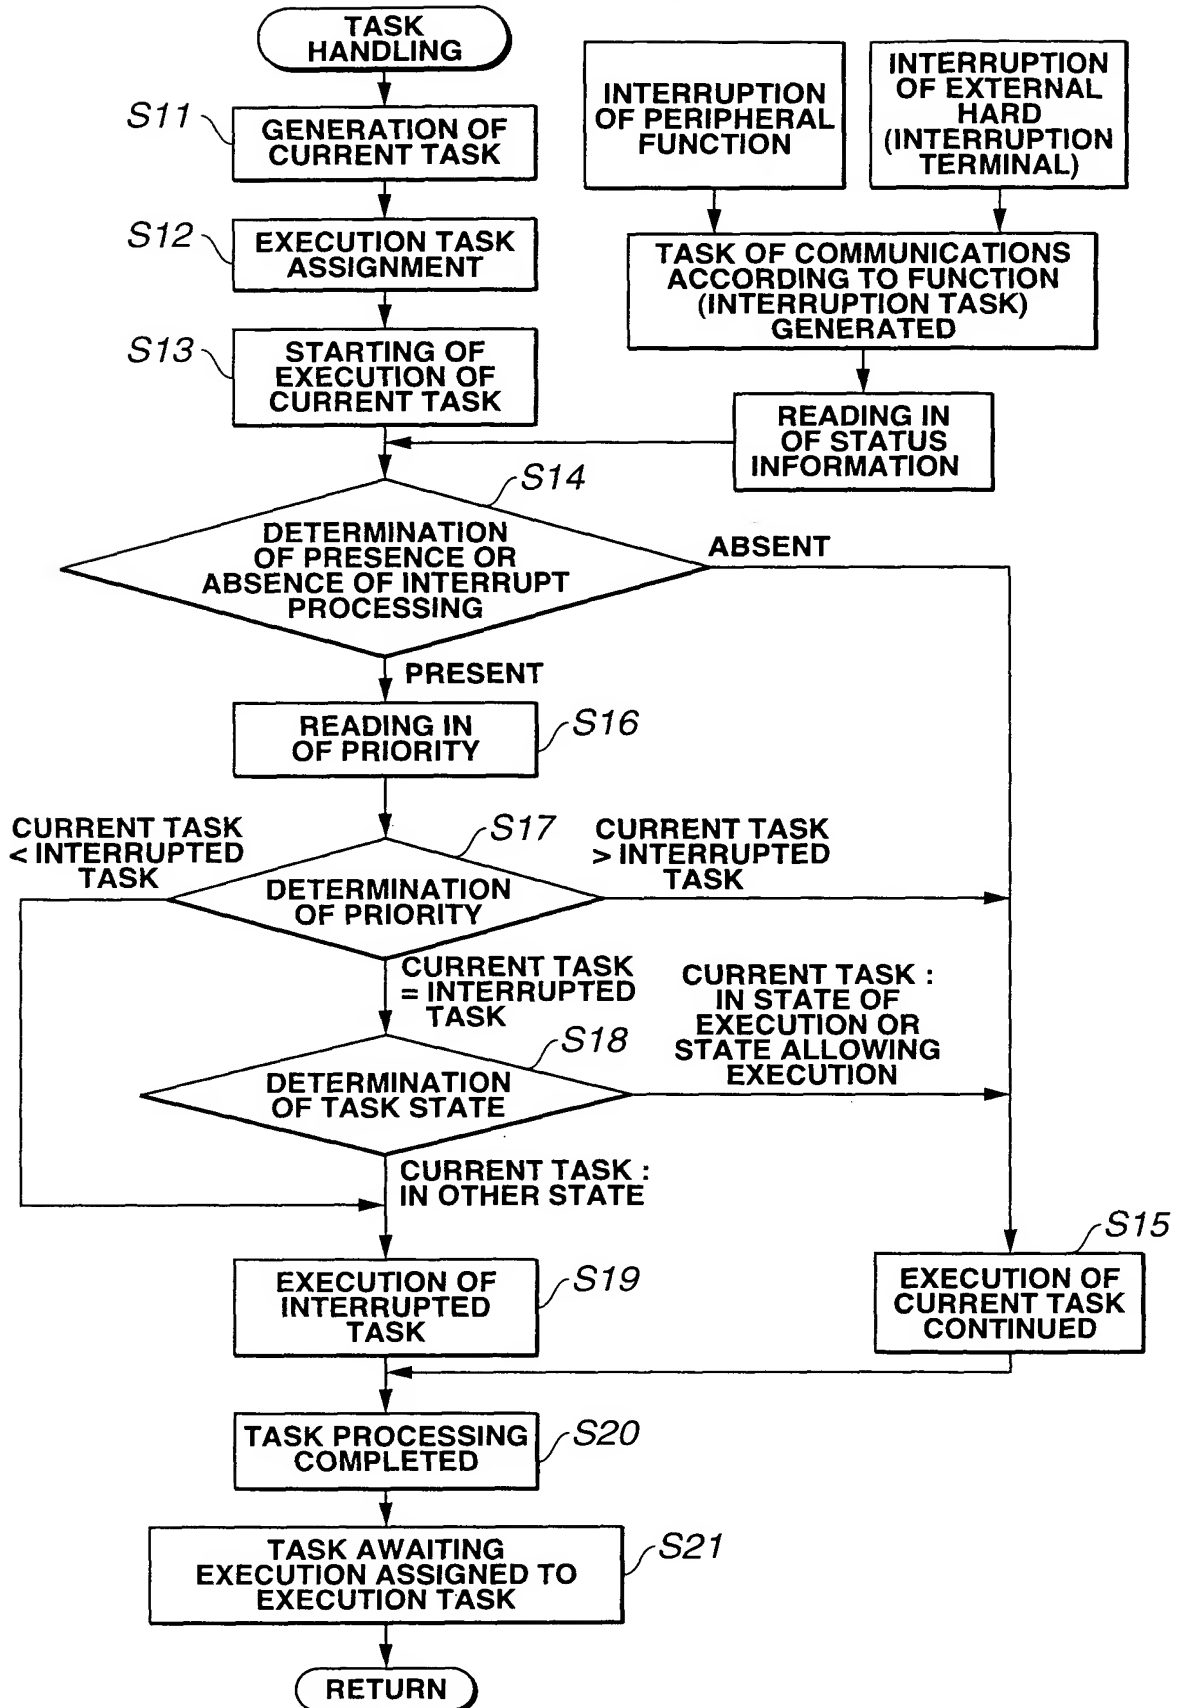


FIG.17

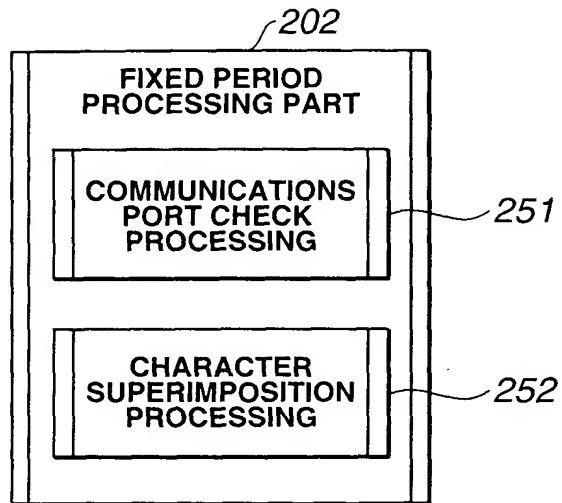


FIG.18

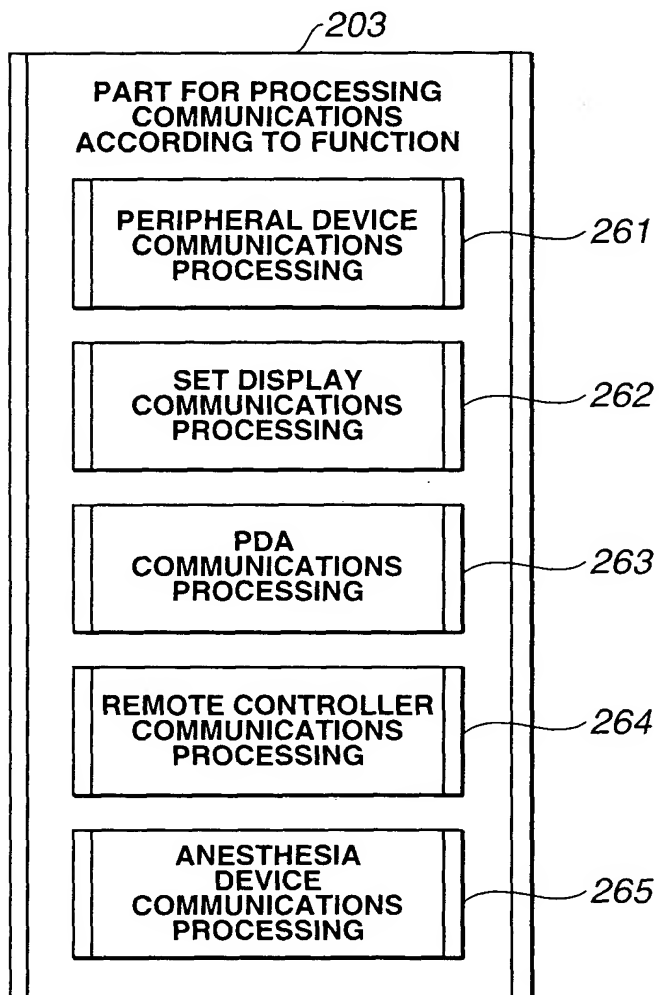


FIG.19

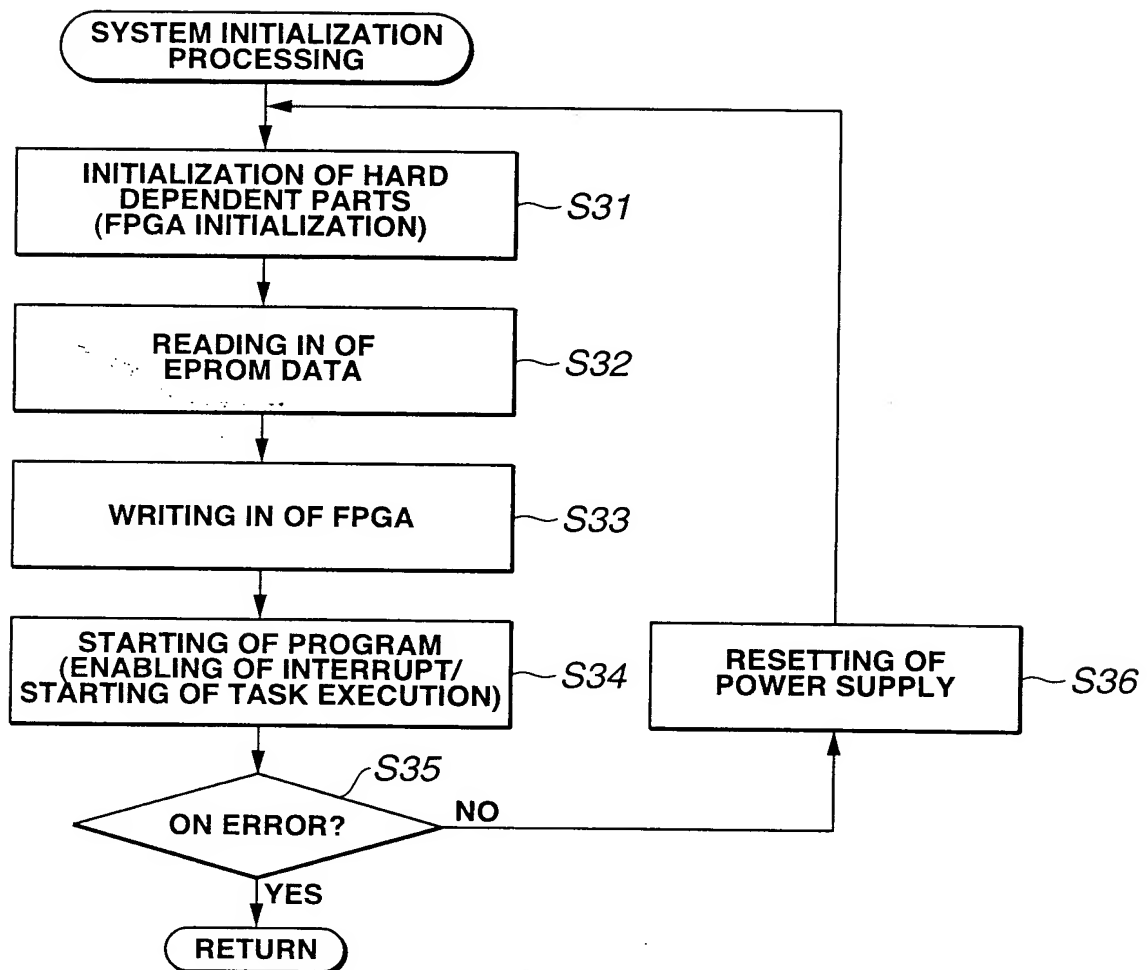


FIG.20

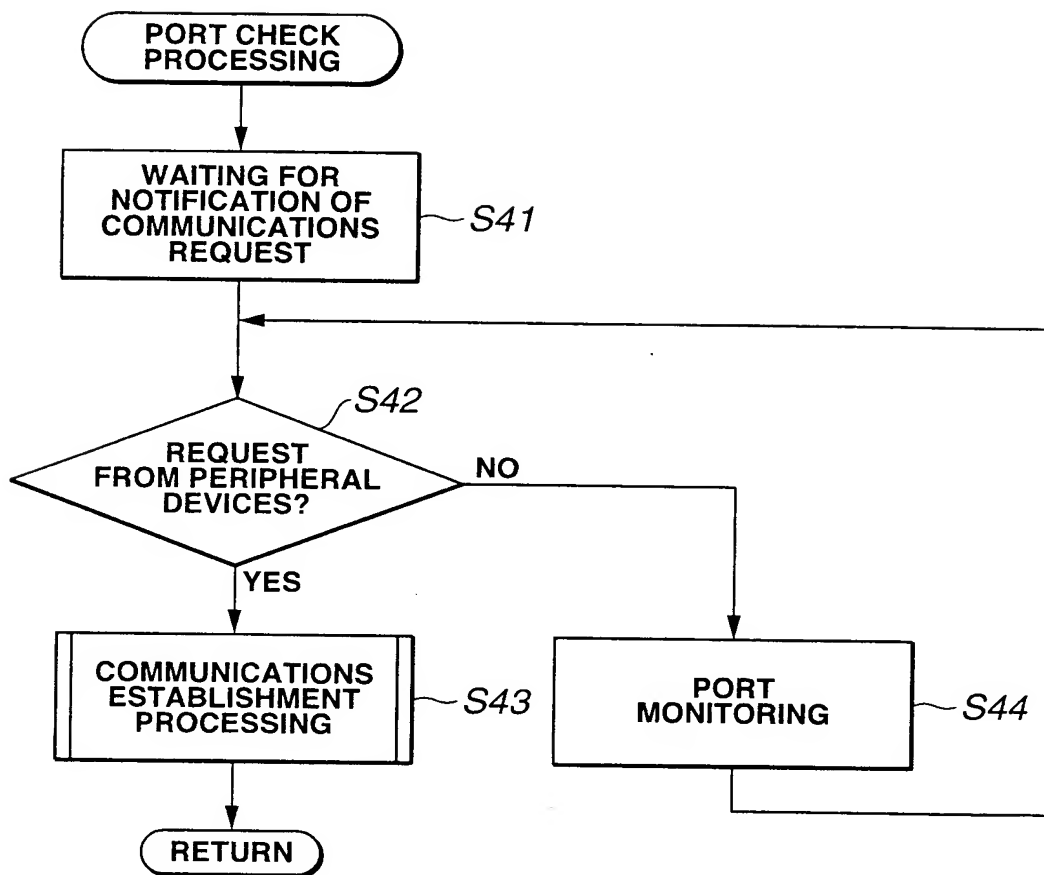


FIG.21

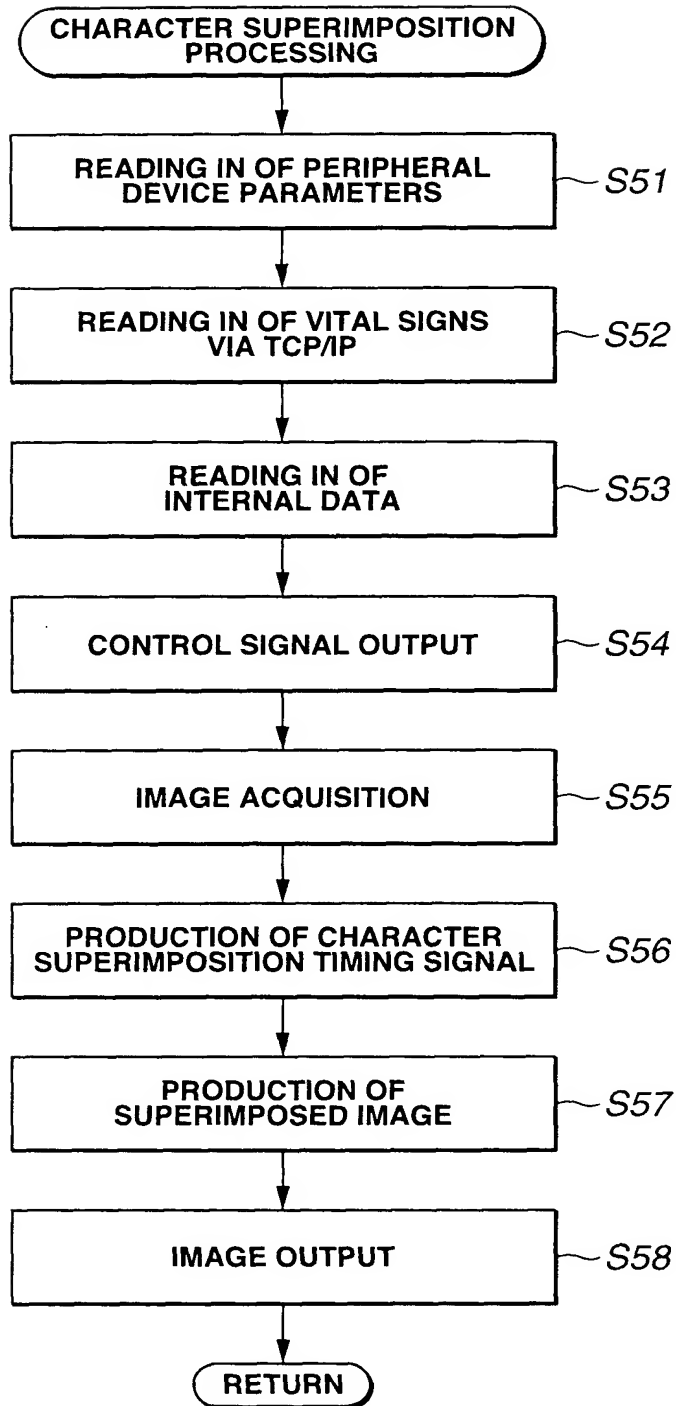


FIG.22

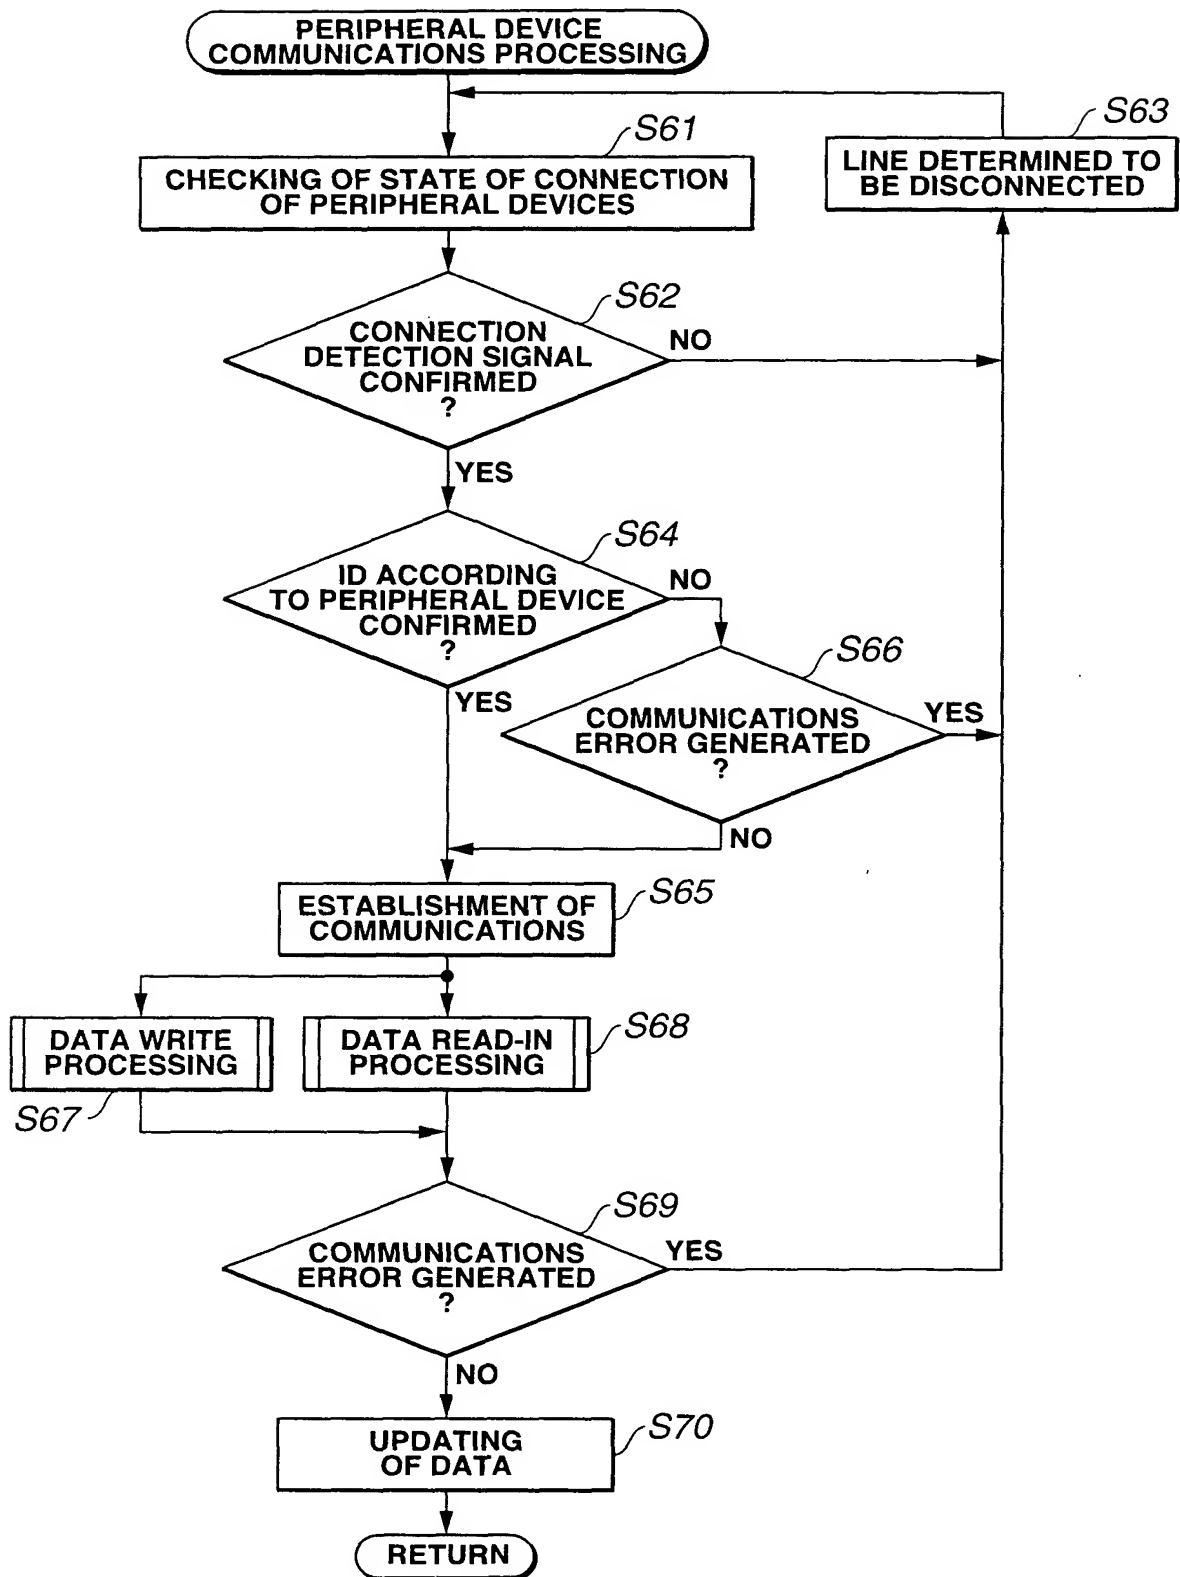


FIG.23

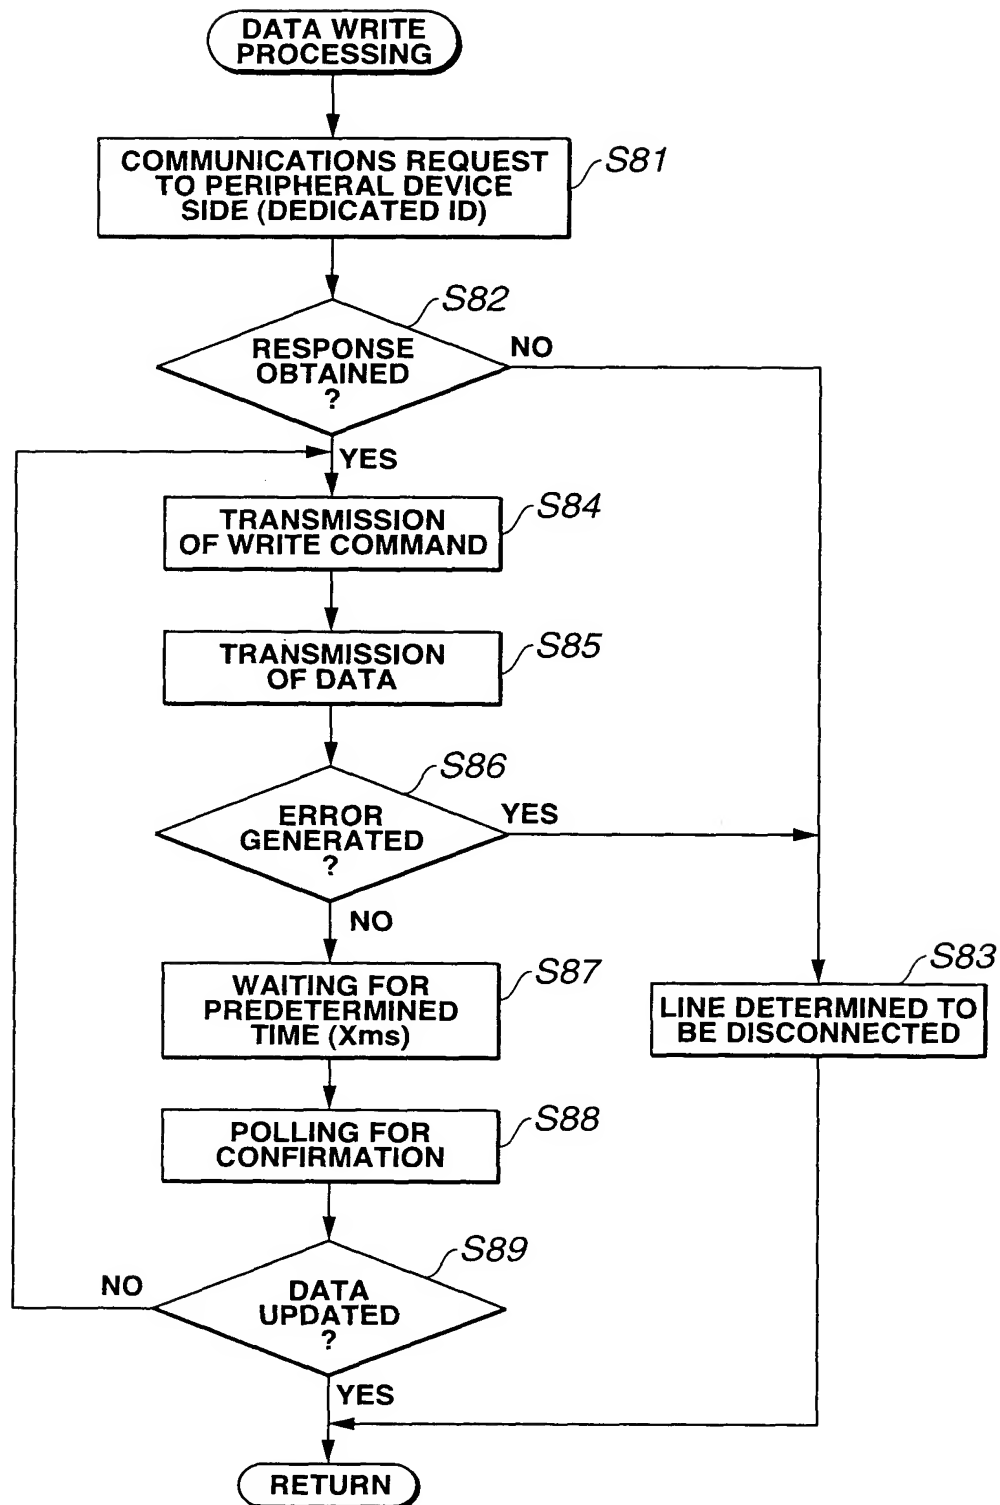


FIG.24

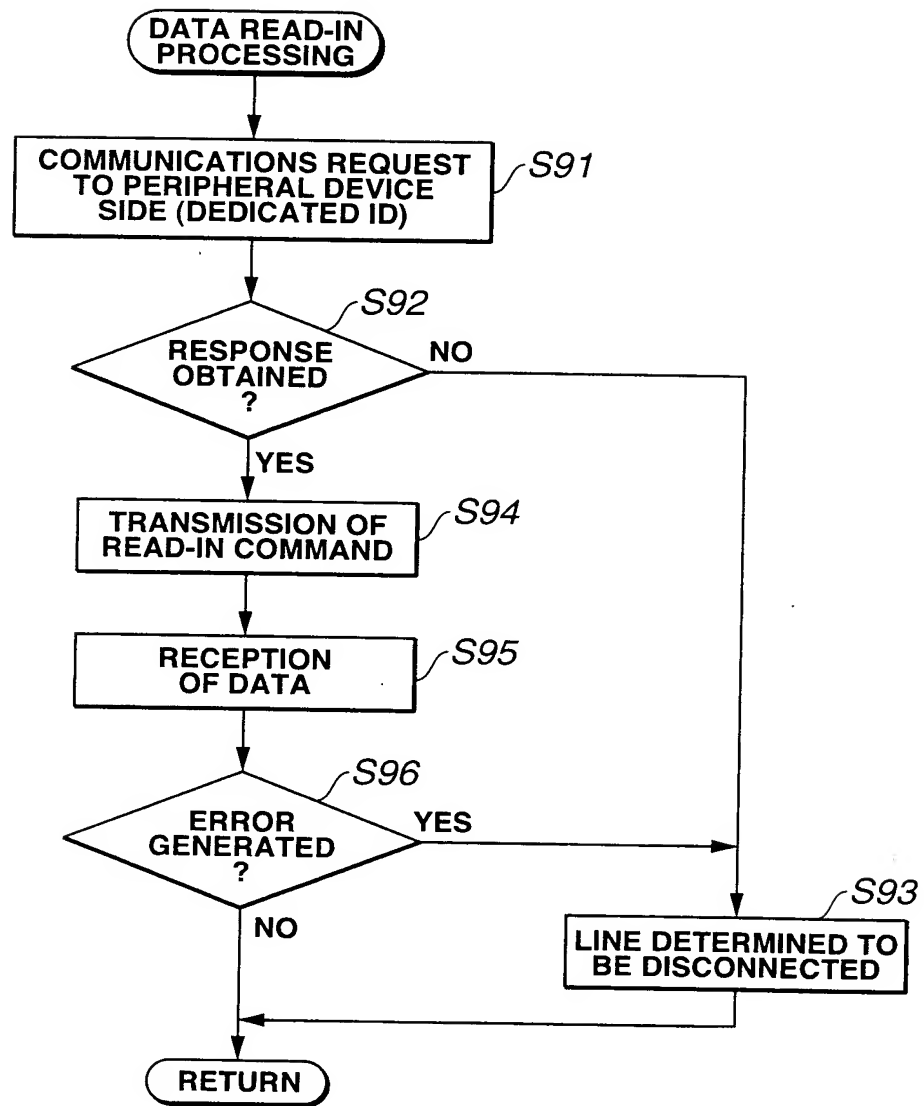


FIG.25

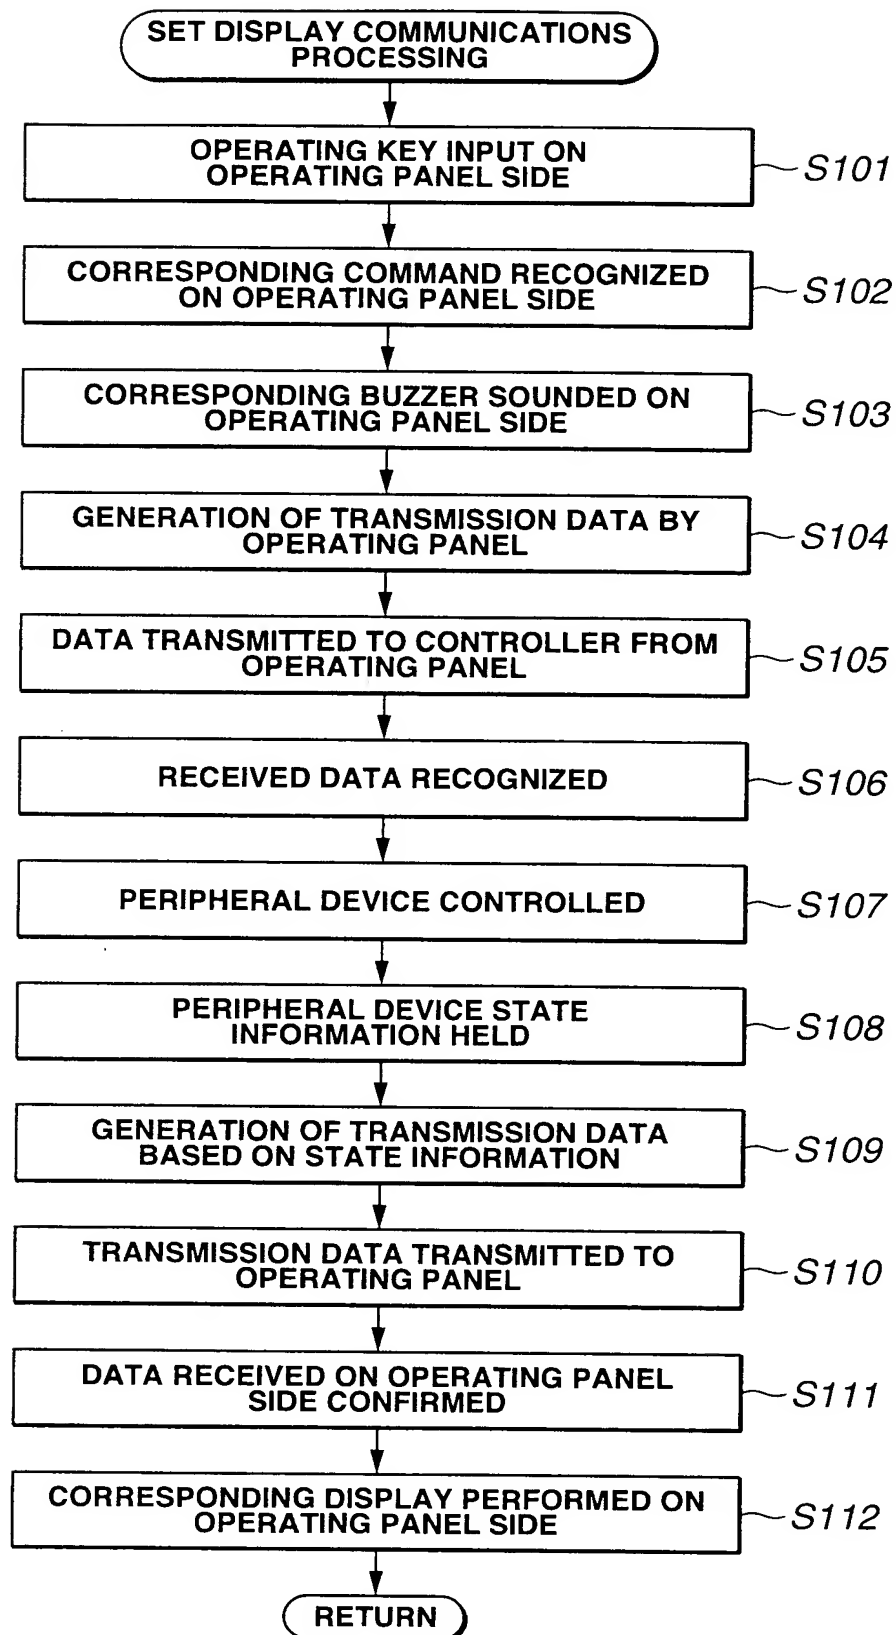


FIG.26

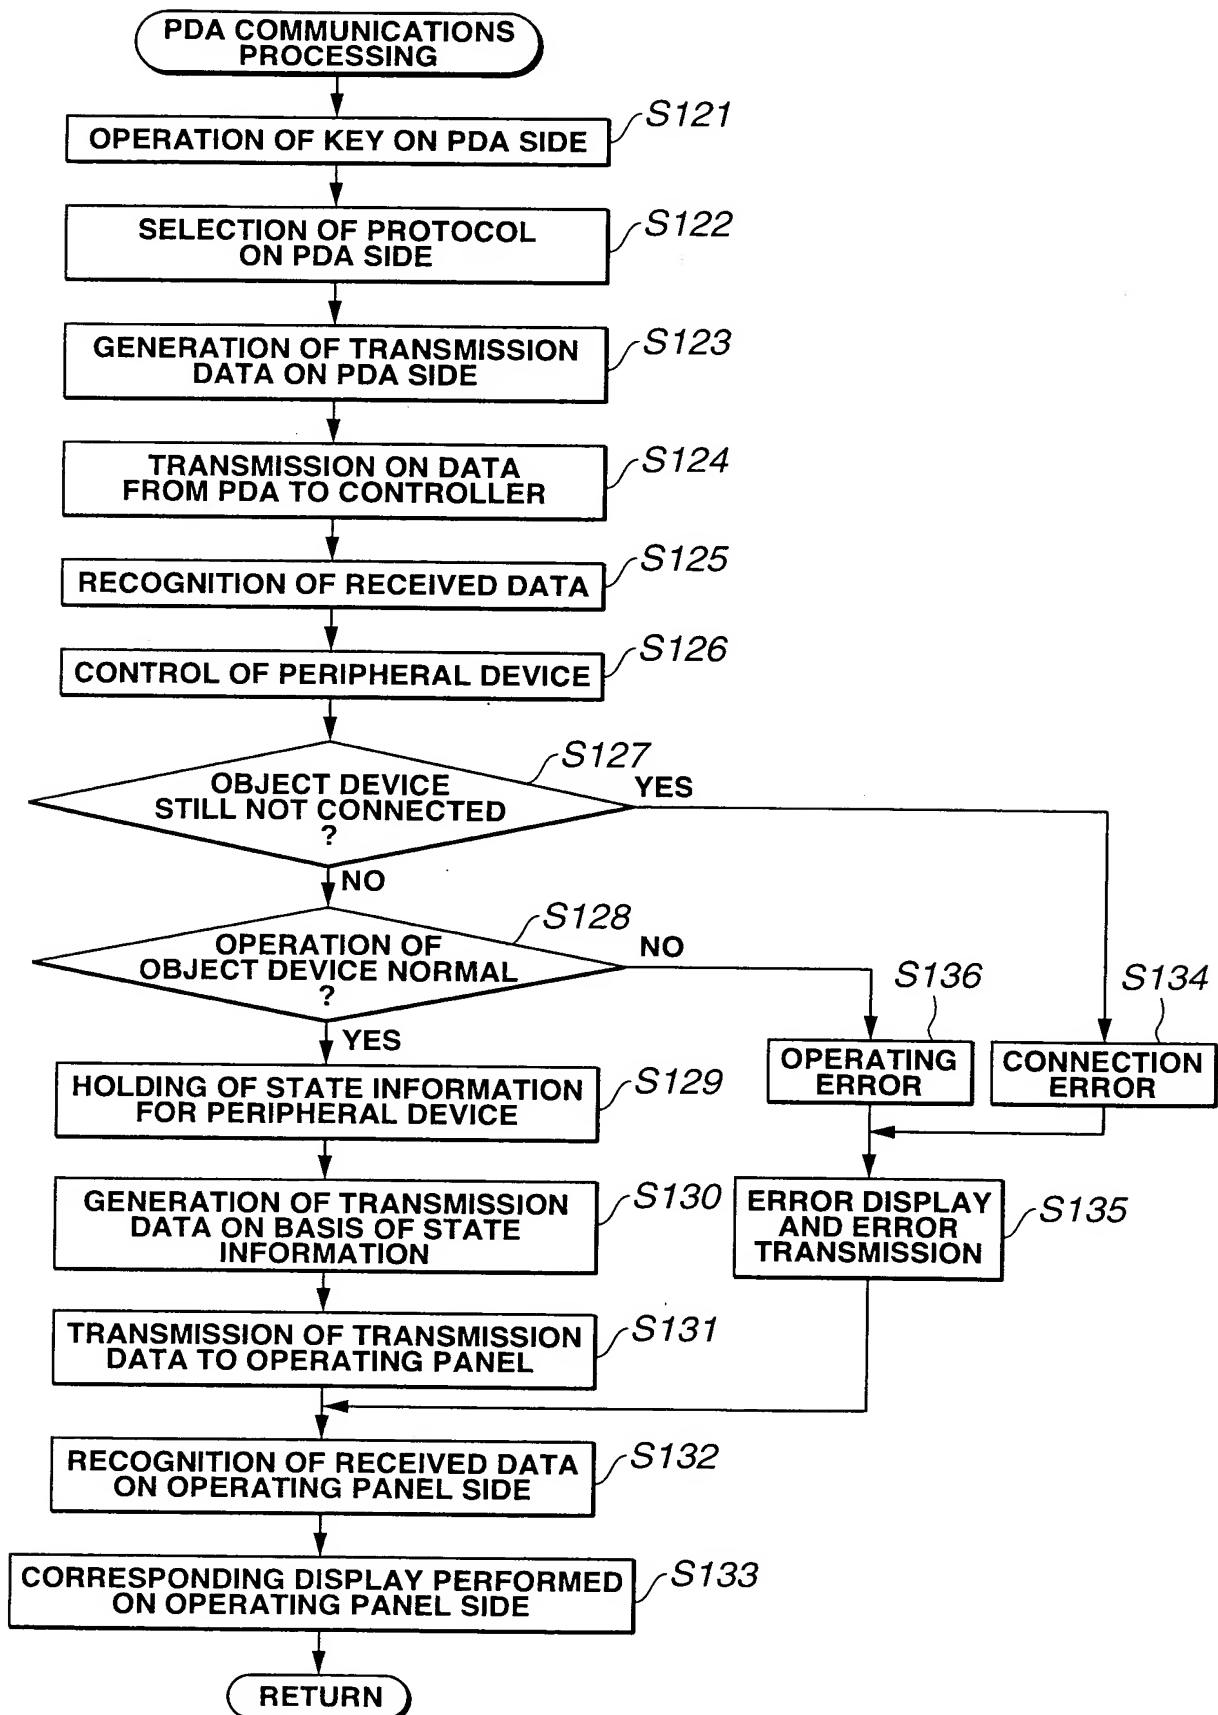


FIG.27

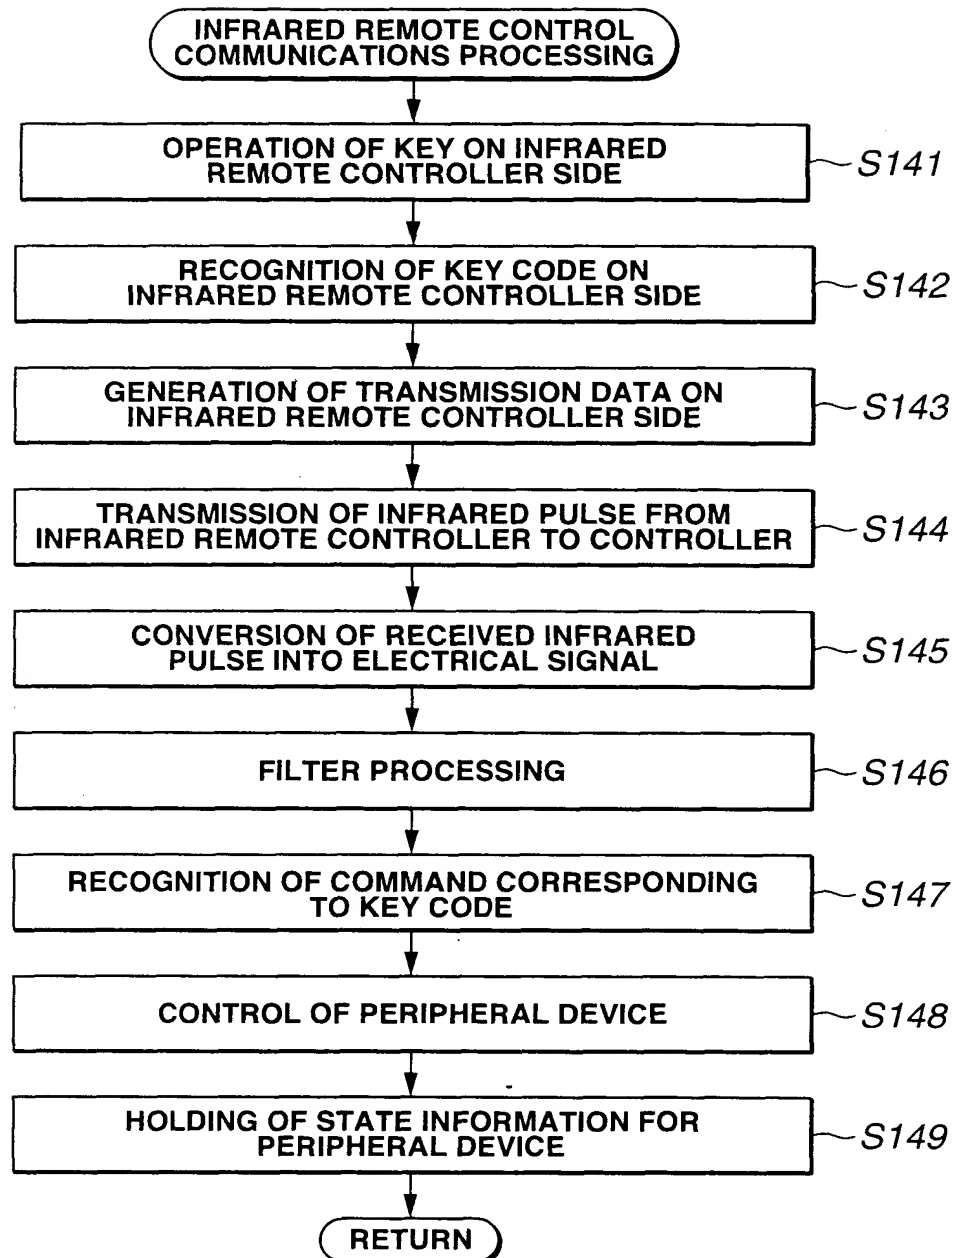


FIG.28

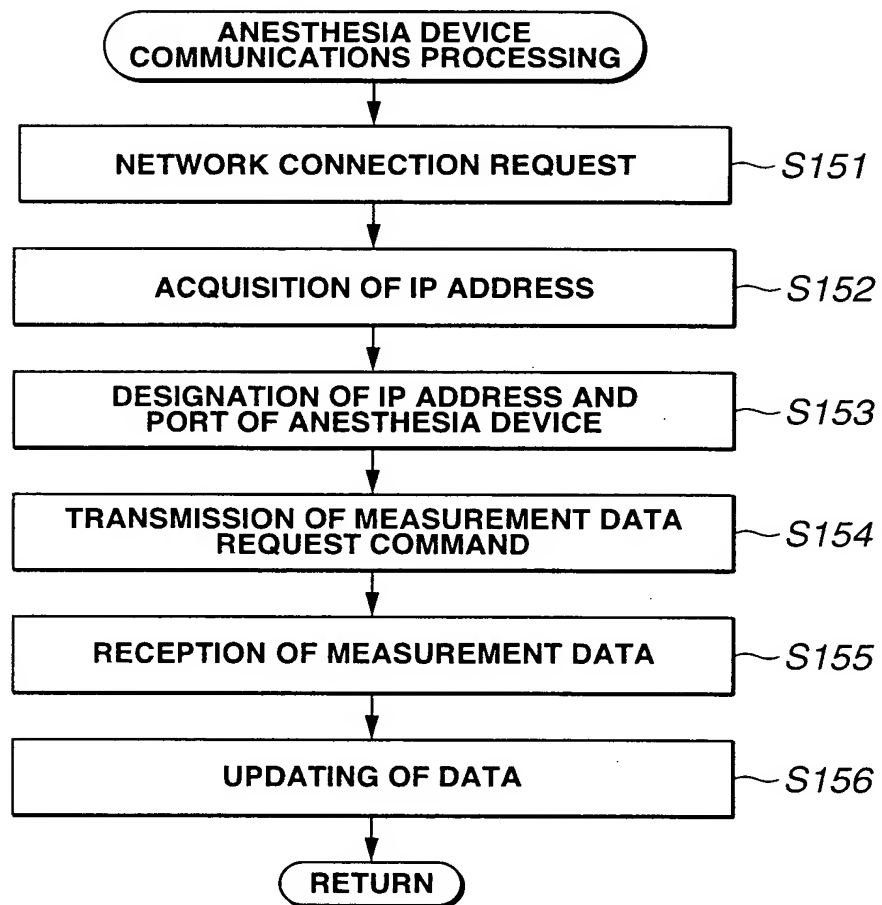


FIG.29

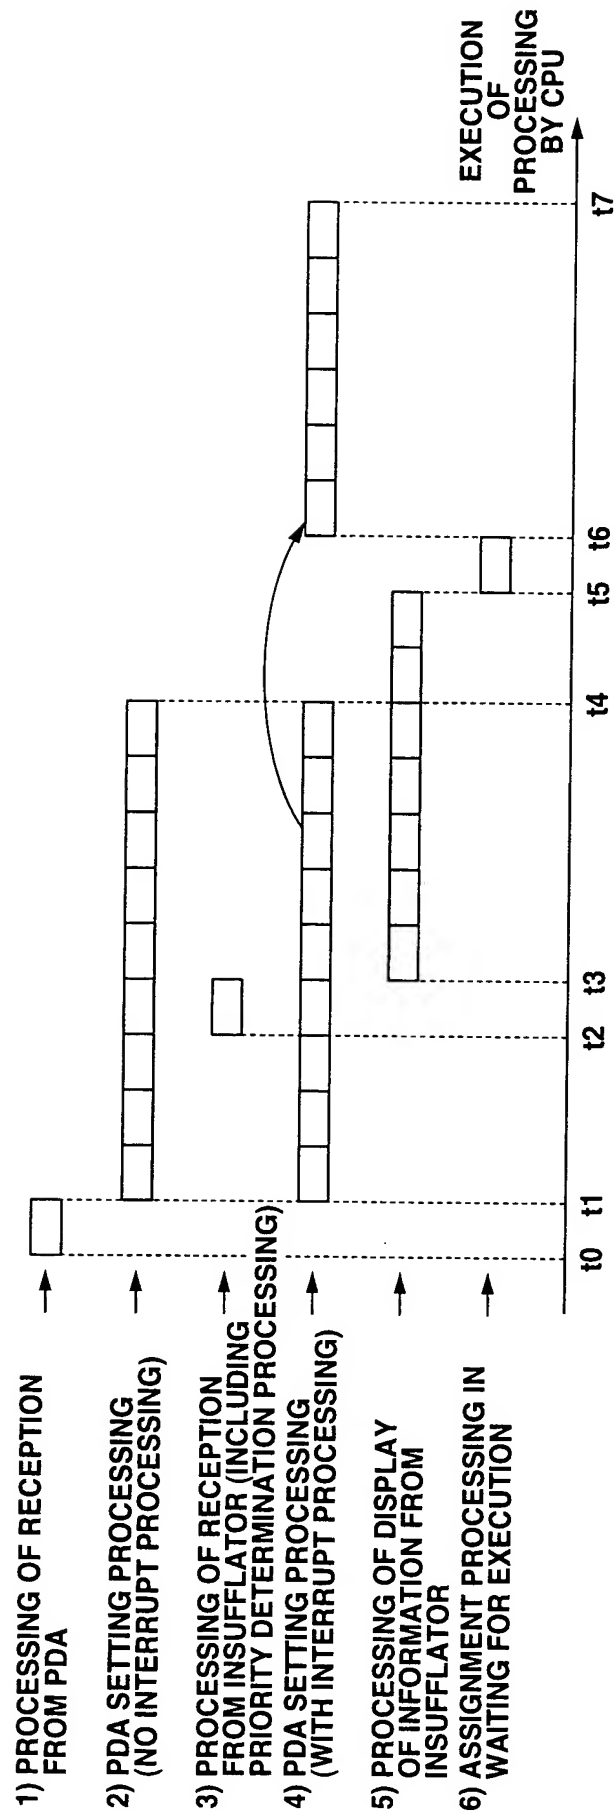


FIG.30

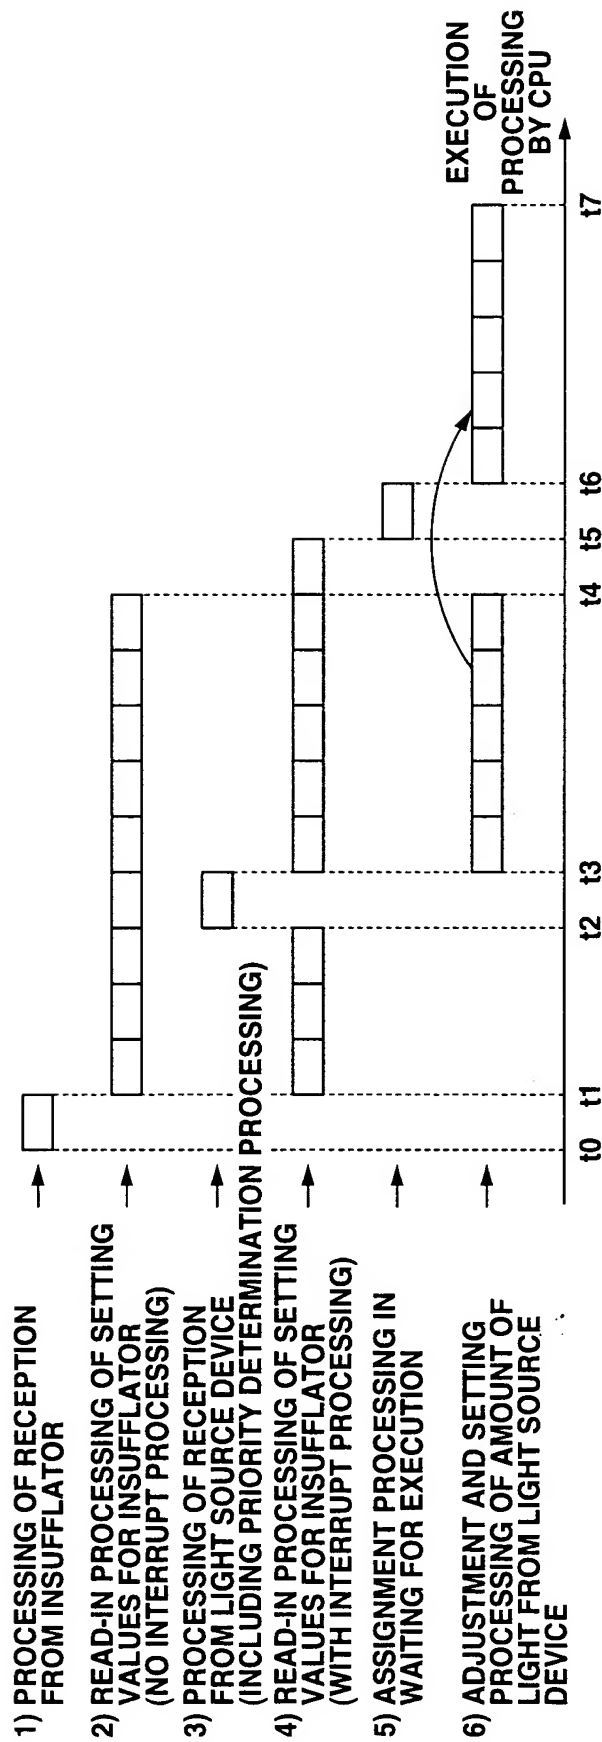


FIG.31

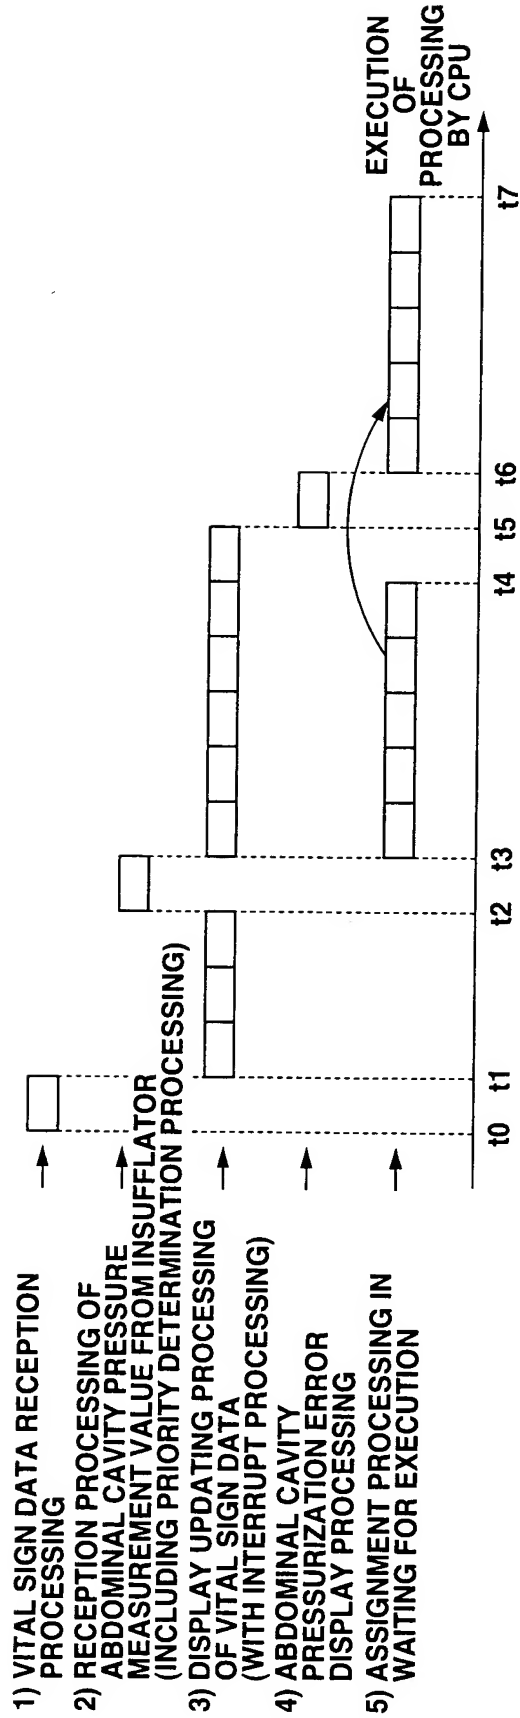


FIG. 32

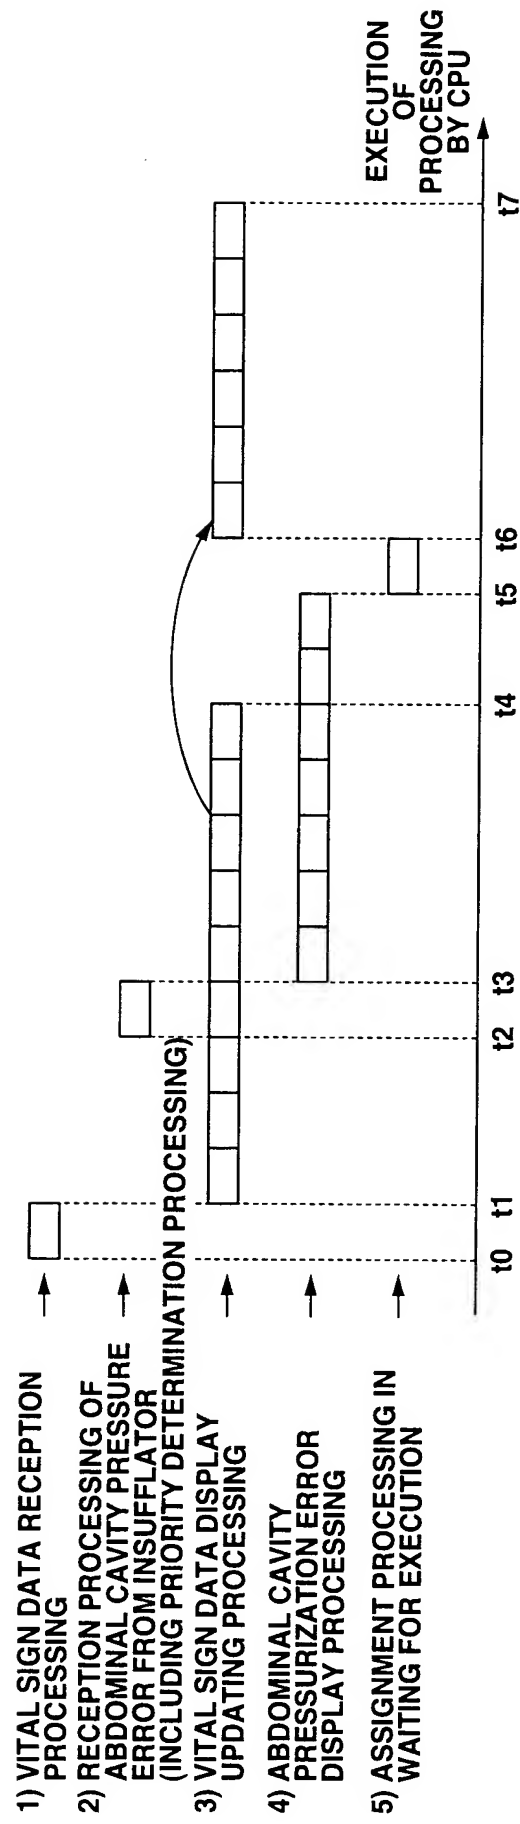


FIG.33

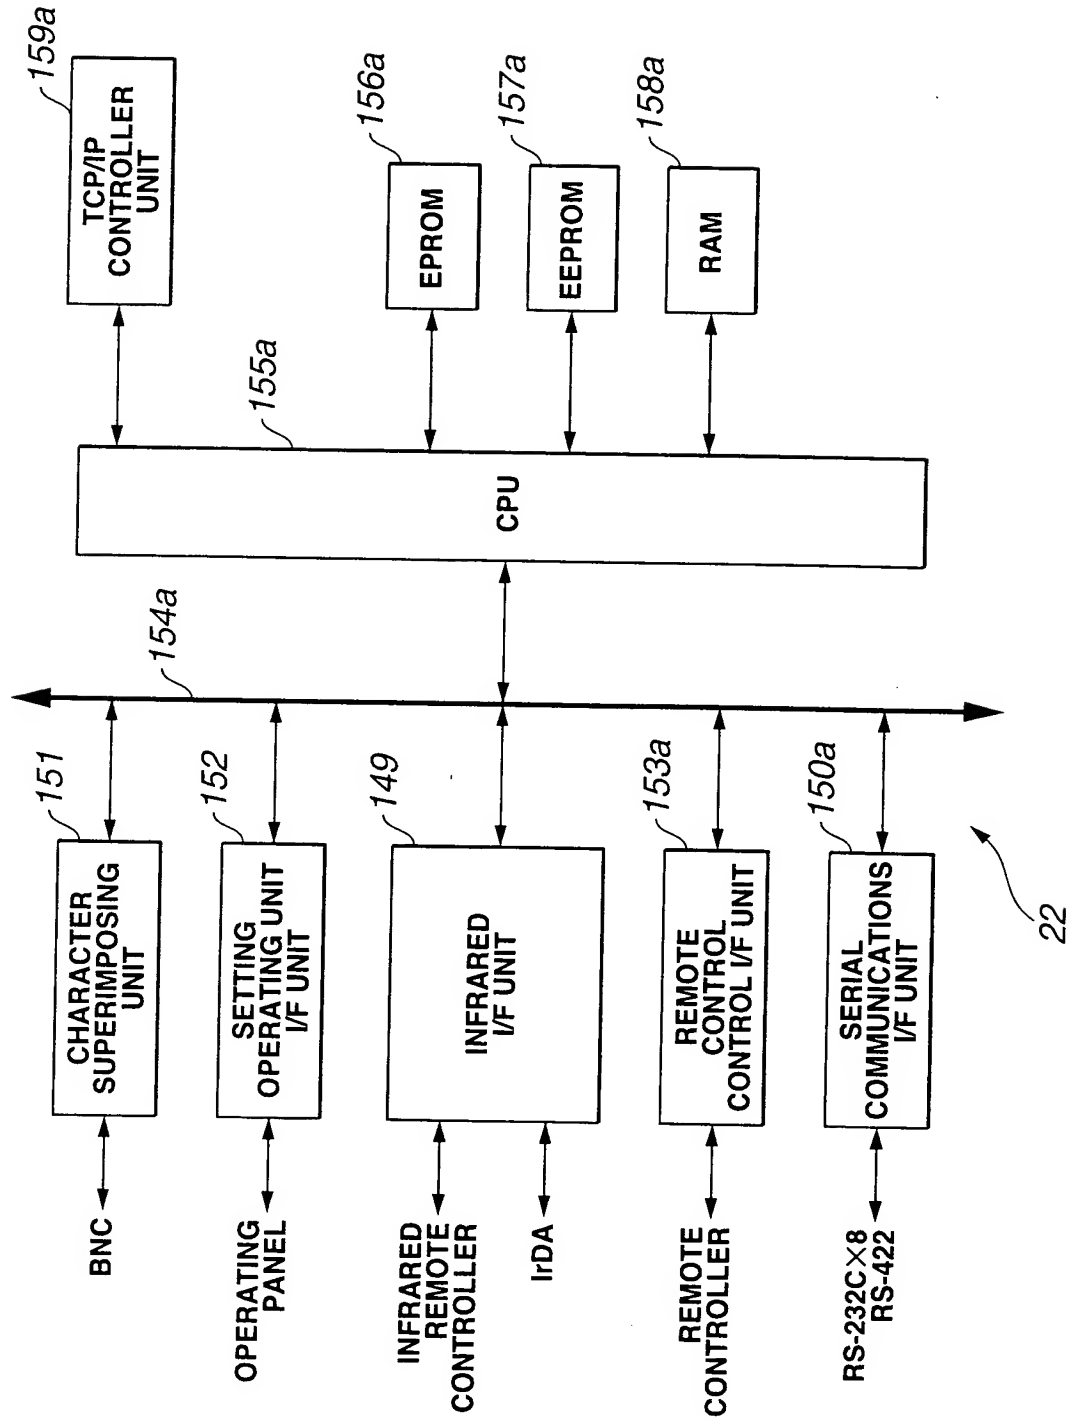


FIG.34

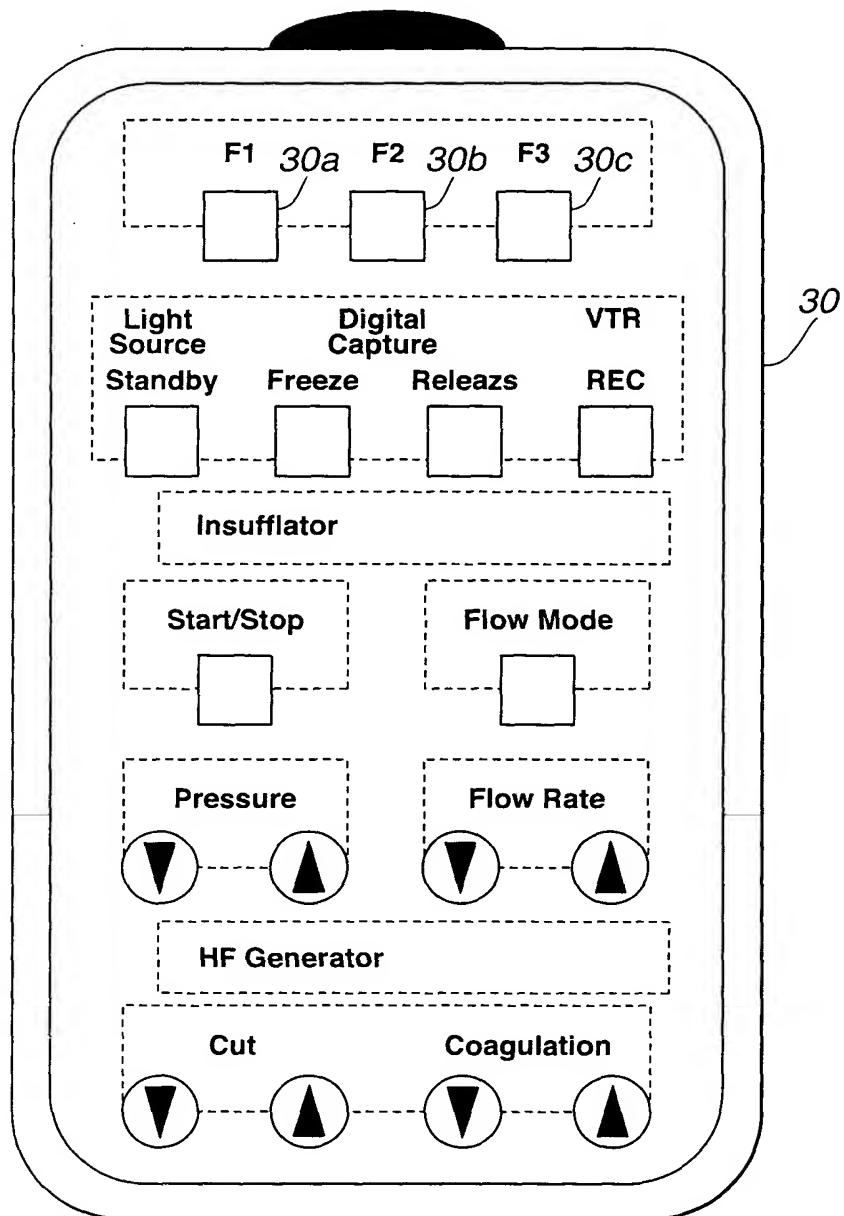


FIG.35

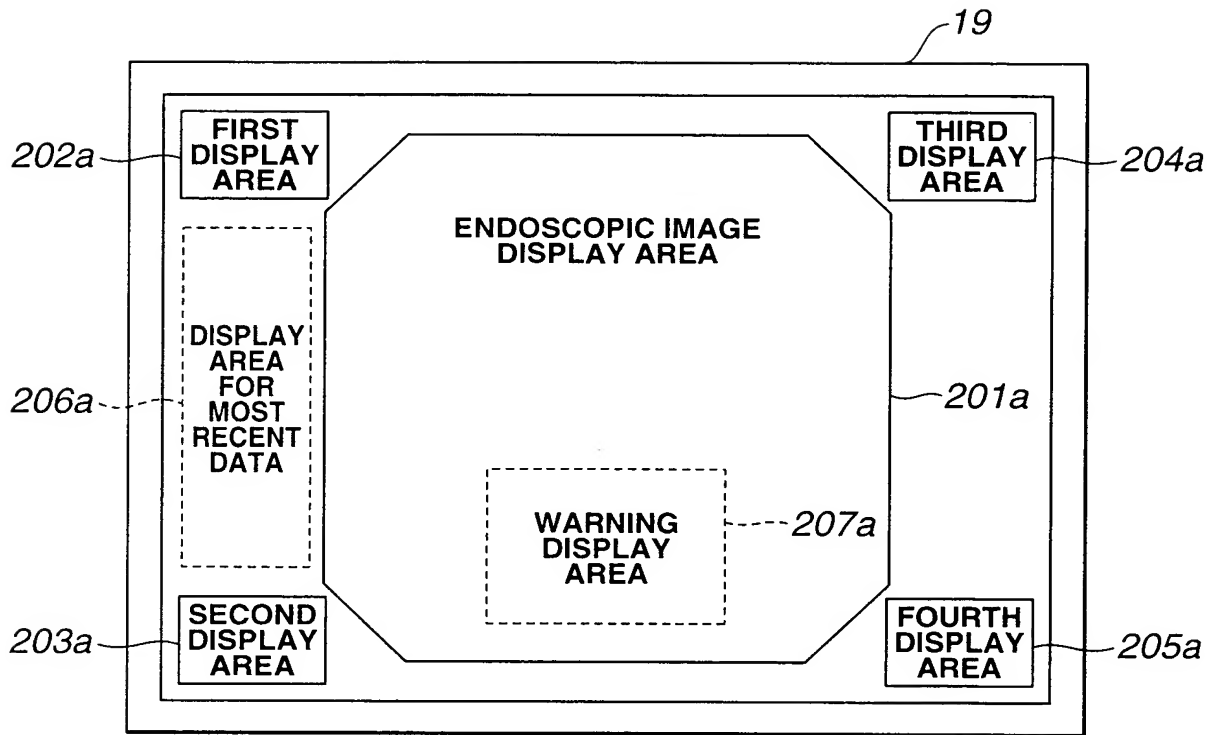


FIG.36

DISPLAY PATTERN	FIRST DISPLAY AREA	SECOND DISPLAY AREA	THIRD DISPLAY AREA	FOURTH DISPLAY AREA
1	——	FLOW RATE	——	ABDOMINAL CAVITY PRESSURE
2	SpO2	FLOW RATE	BLOOD PRESSURE	ABDOMINAL CAVITY PRESSURE
3	PULSE	FLOW RATE	BLOOD PRESSURE	ABDOMINAL CAVITY PRESSURE
4	BODY TEMPERATURE	FLOW RATE	BLOOD PRESSURE	ABDOMINAL CAVITY PRESSURE

FIG.37

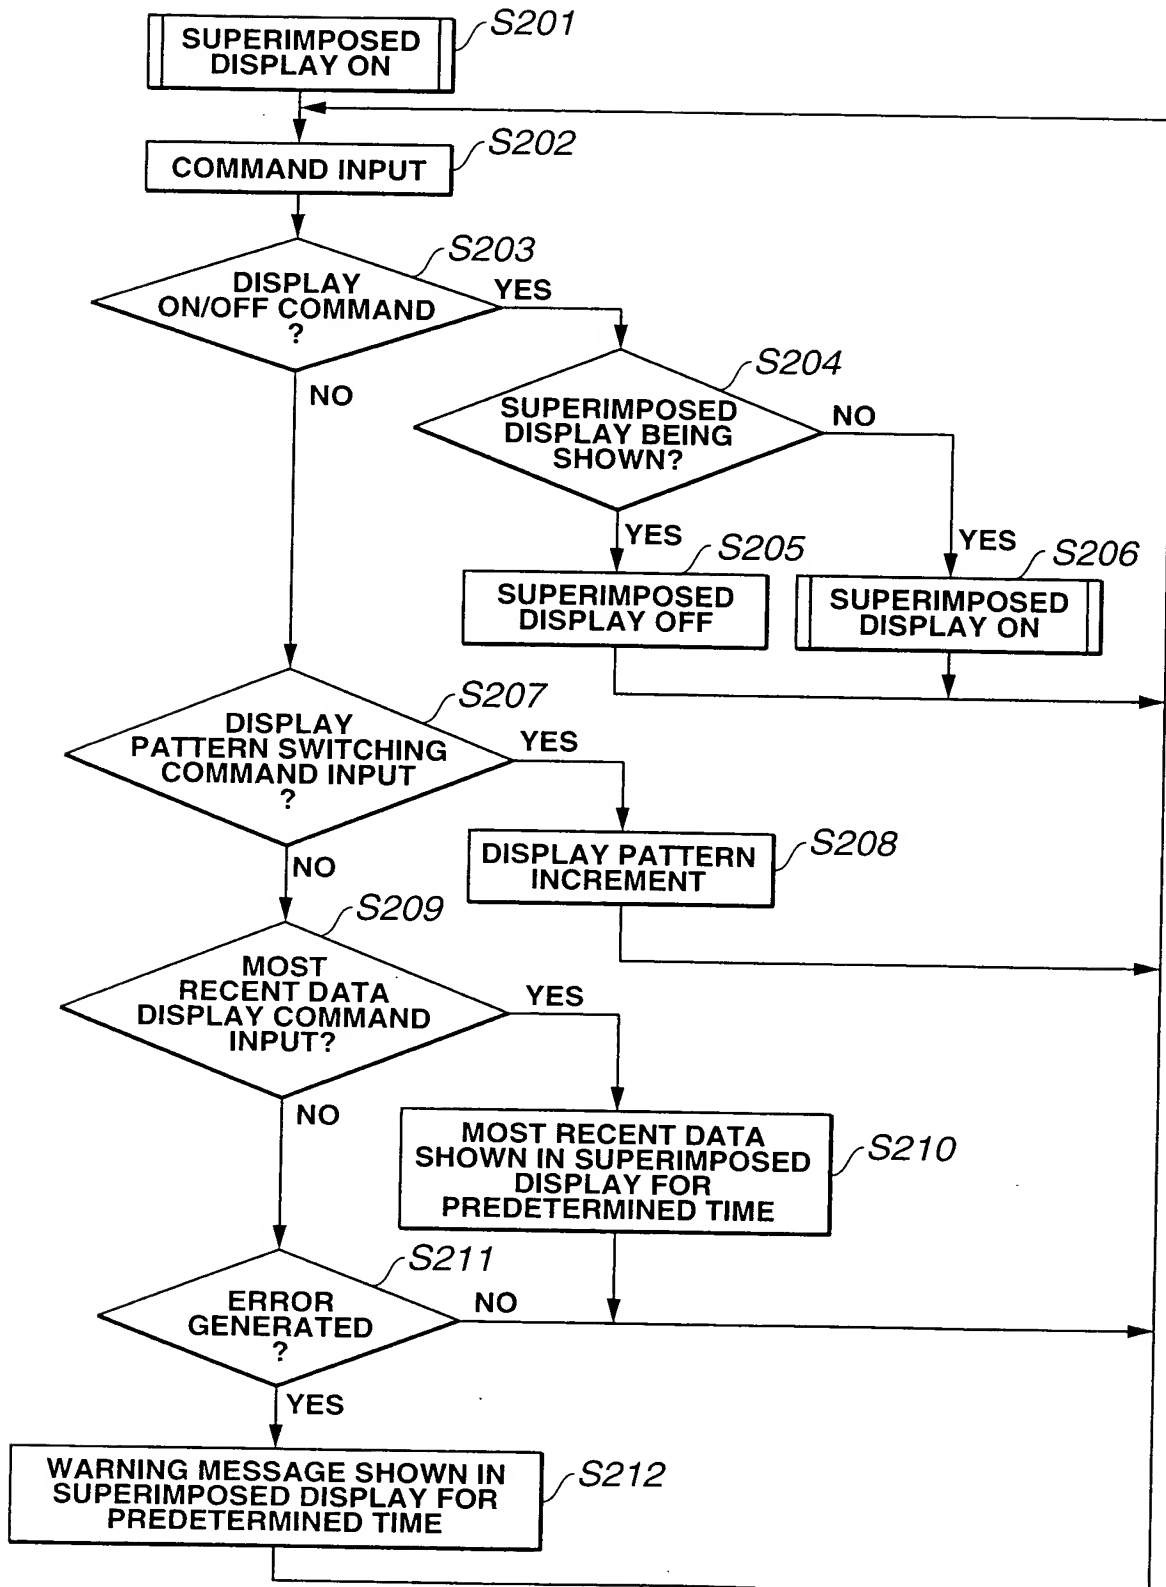


FIG.38

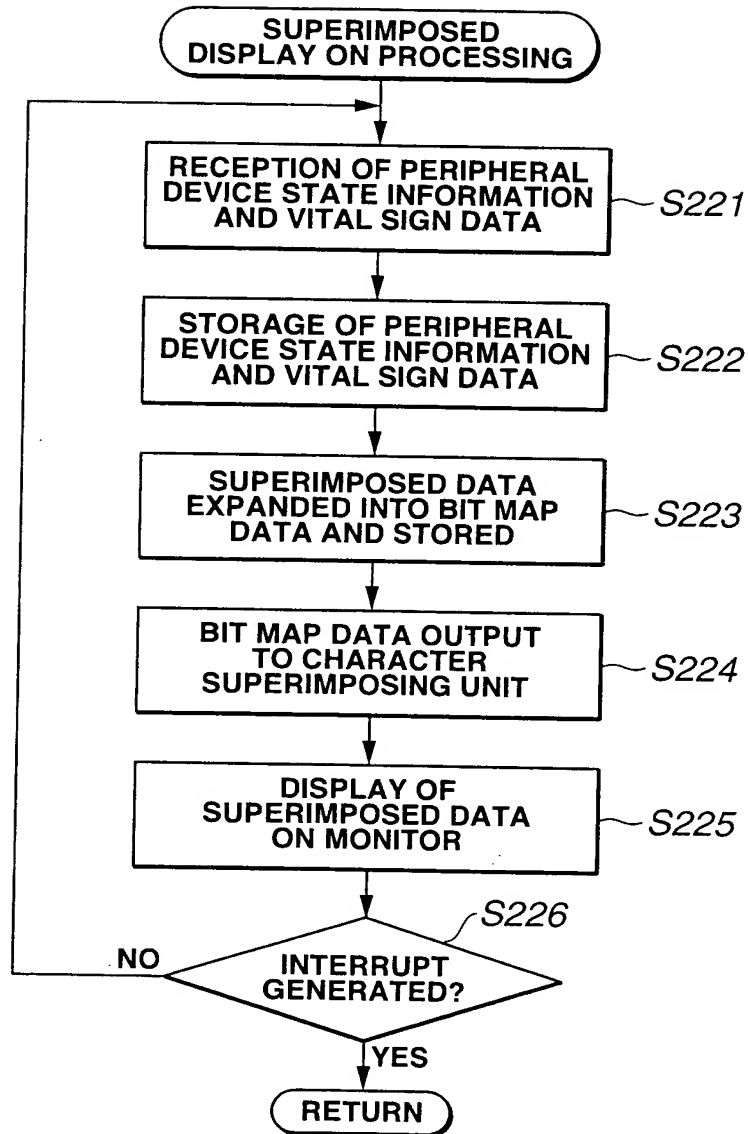


FIG.39

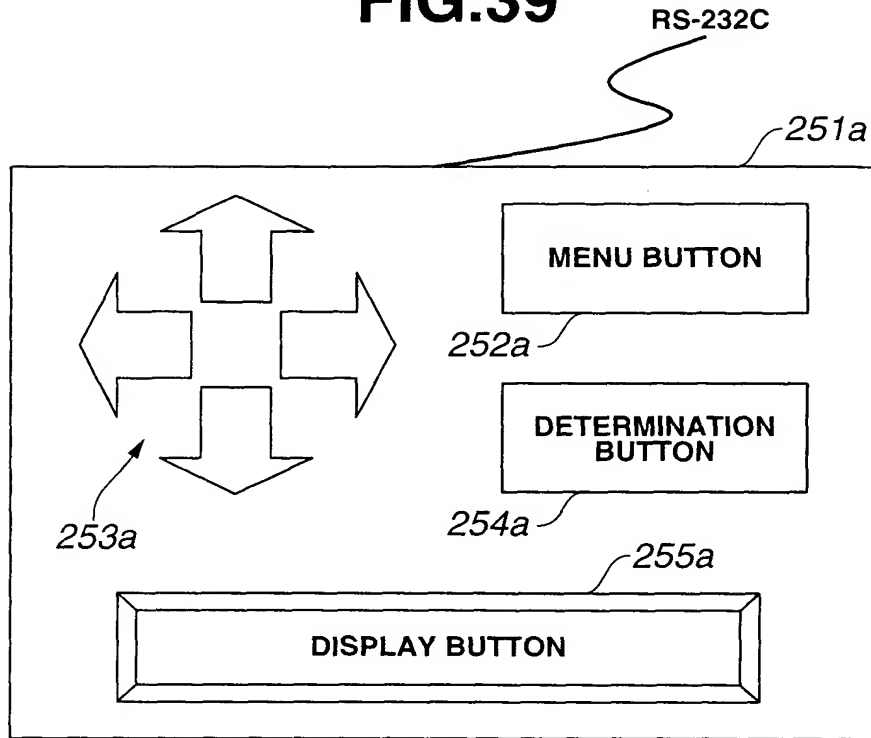


FIG.40

19

SUPERIMPOSED DATA SETTING SCREEN

(1) SUPERIMPOSED DISPLAY ☐ ON / OFF

(2) DISPLAY MODE ☐ PERMANENT DISPLAY / ☐ DISPLAY FOR PREDETERMINED TIME

(3) DISPLAY PATTERN 1 / 2 / 3 / 4

(4) DISPLAY PATTERN ATTRIBUTE SETTING

	FIRST DISPLAY AREA	FIRST DISPLAY AREA	FIRST DISPLAY AREA	FIRST DISPLAY AREA
PARAMETER	▼ BODY TEMPERATURE	▼ PULSE	▼ ABDOMINAL CAVITY PRESSURE	▼ NONE
COLOR	▼ WHITE	▼ WHITE	▼ WHITE	▼ YELLOW
SIZE	▼ 10	▼ 10	▼ 10	▼

(5) ERROR DISPLAY ATTRIBUTE SETTING

DISPLAY TIME ▼ 1s

DISPLAY SIZE ▼ 1s

260a

REGISTER

FIG.41

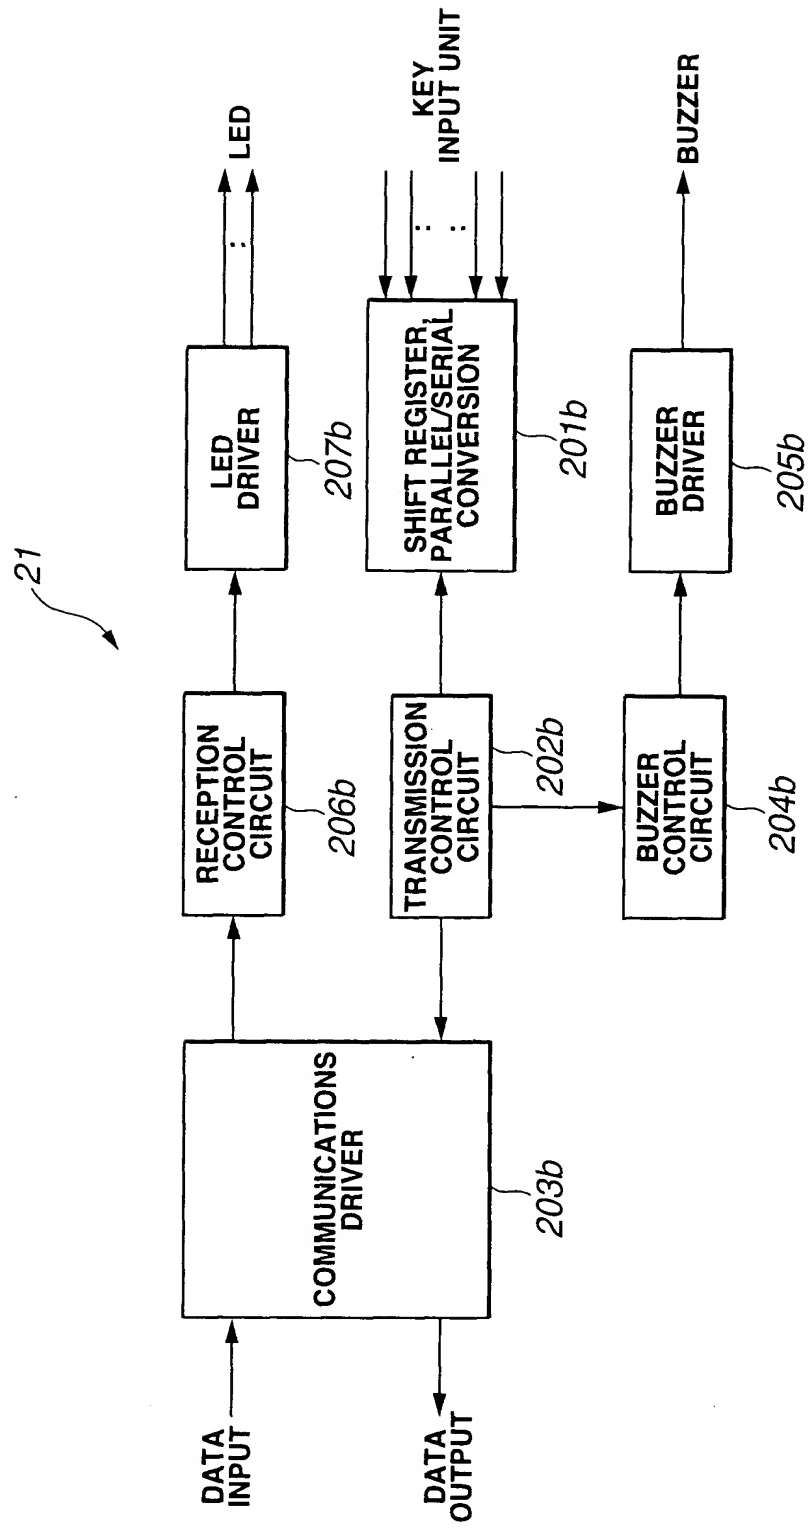


FIG.42

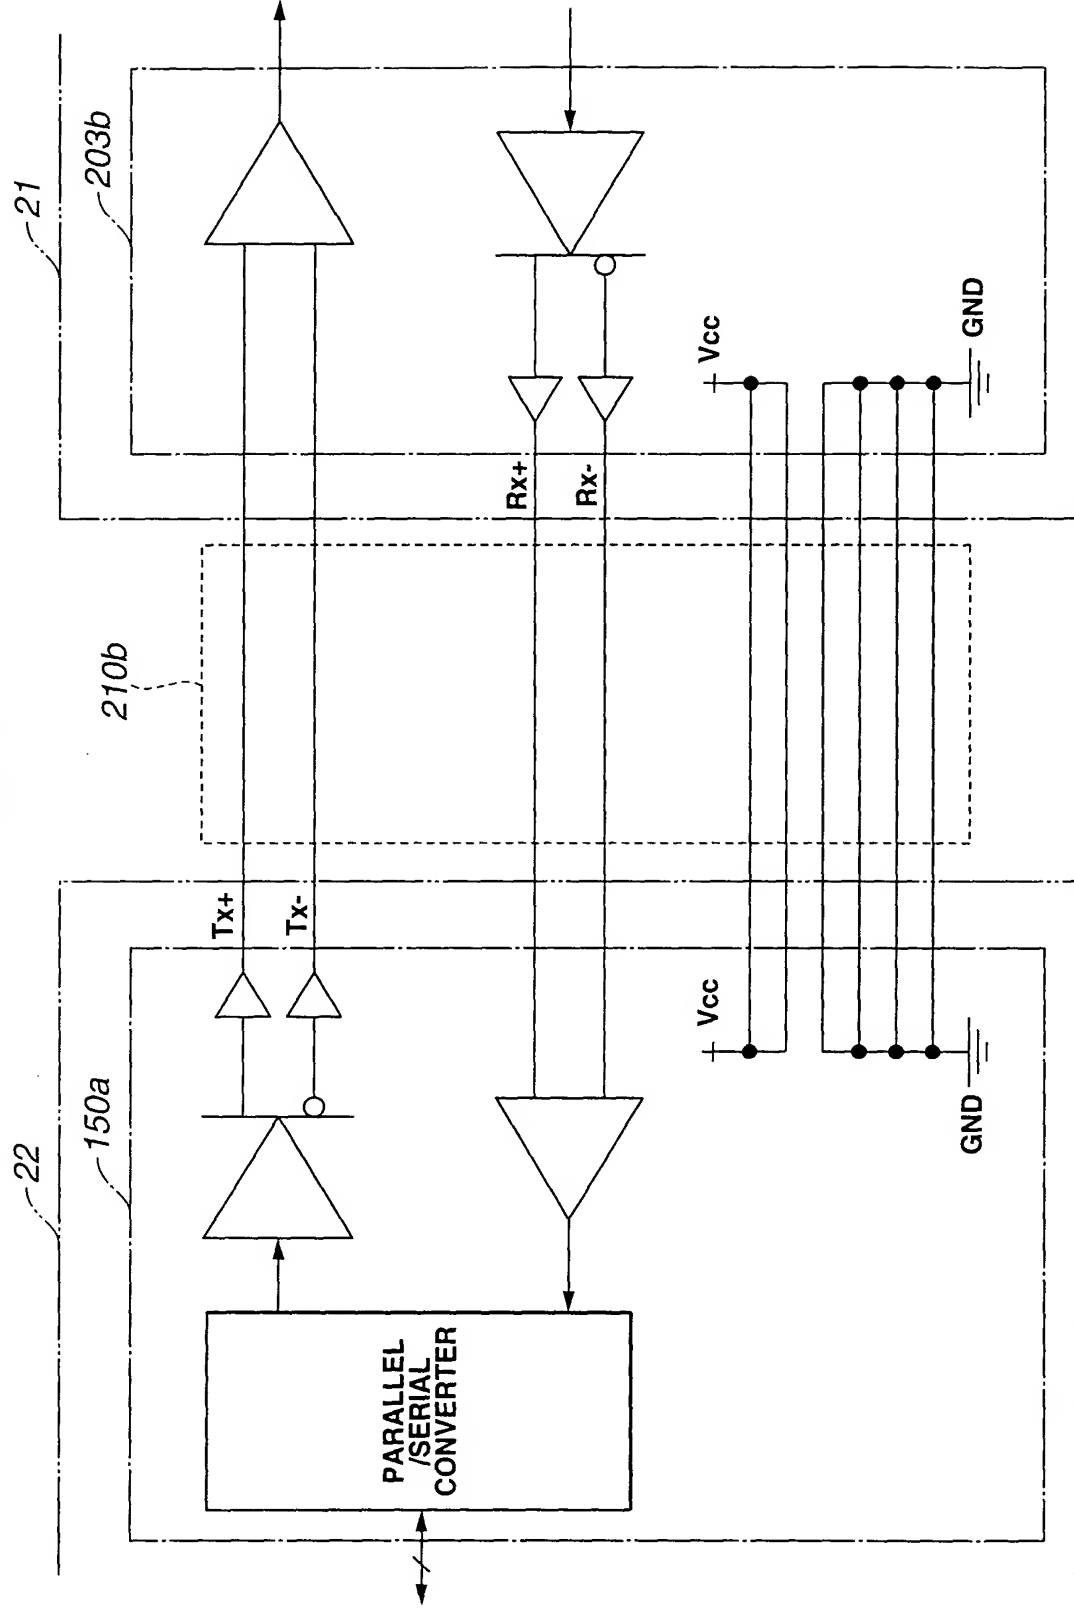


FIG.43

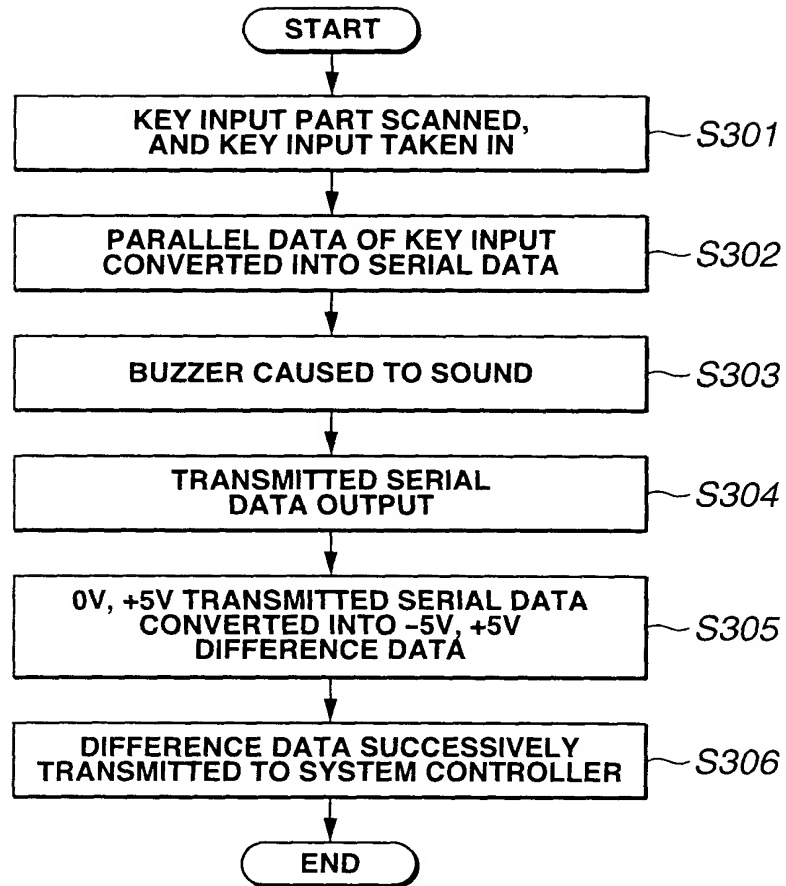


FIG.44

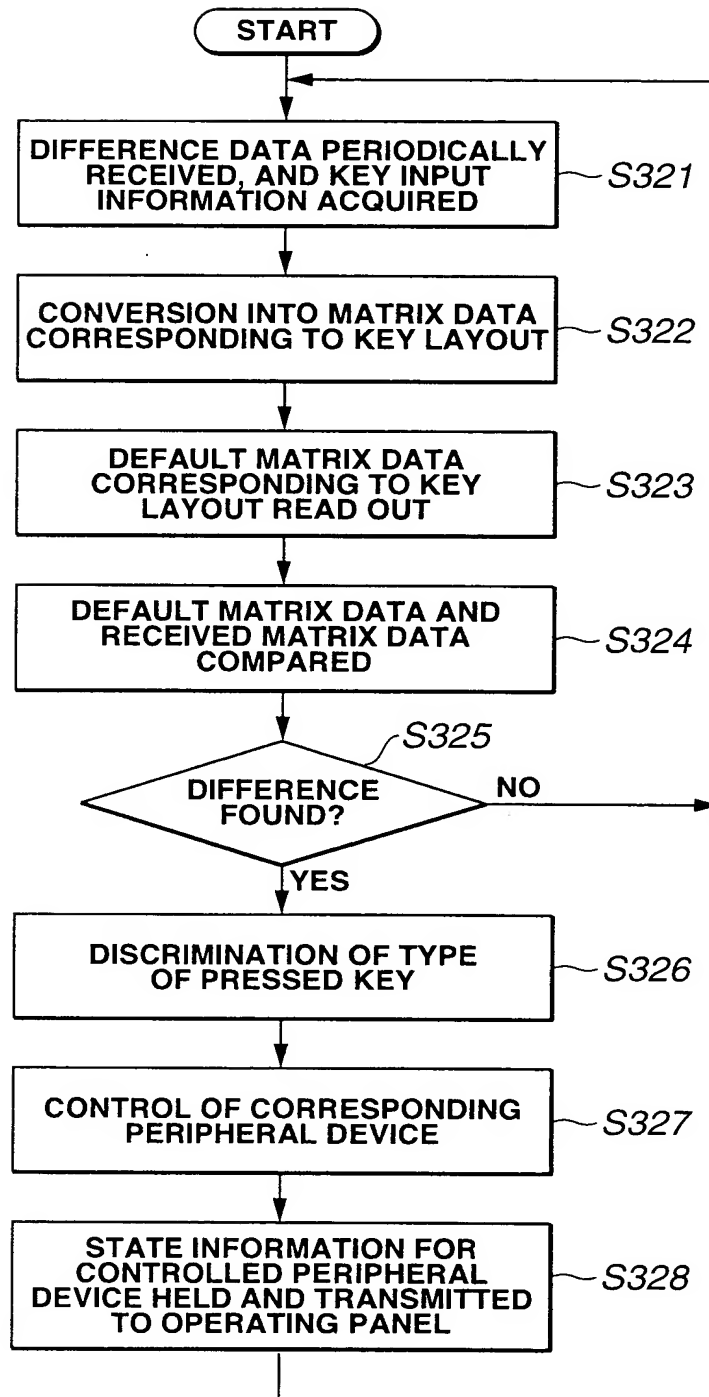


FIG.45

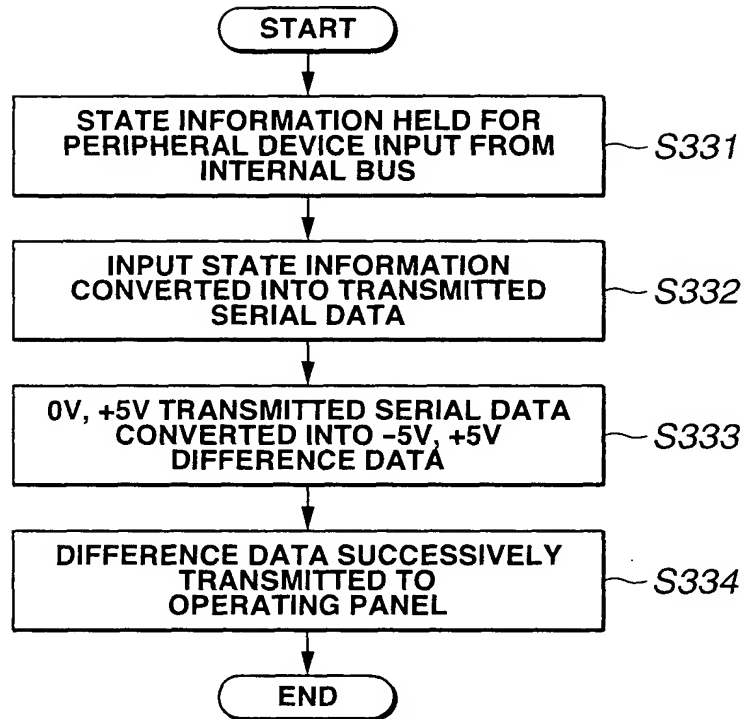


FIG.46

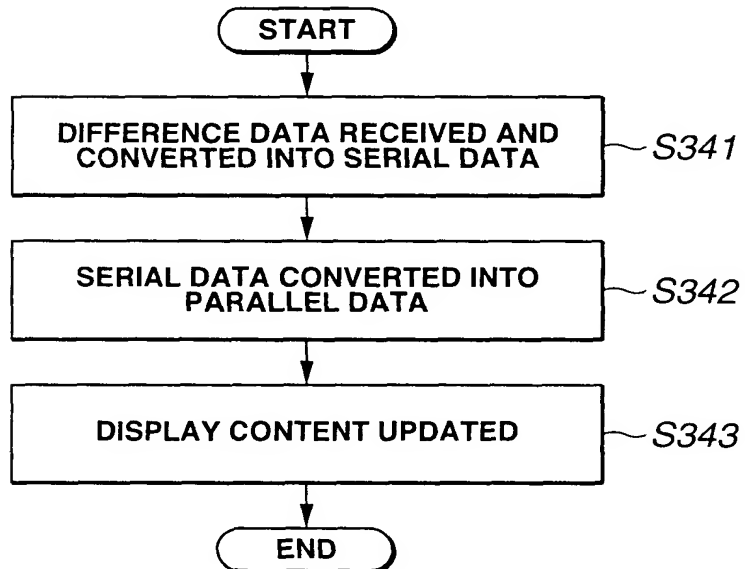


FIG.47

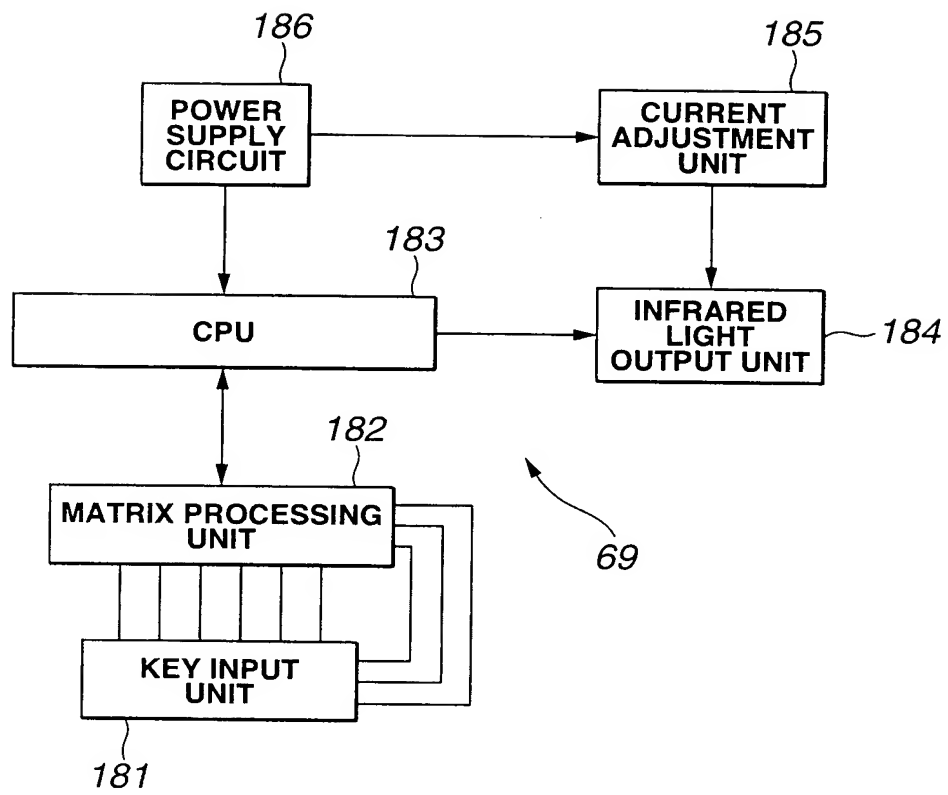


FIG.48

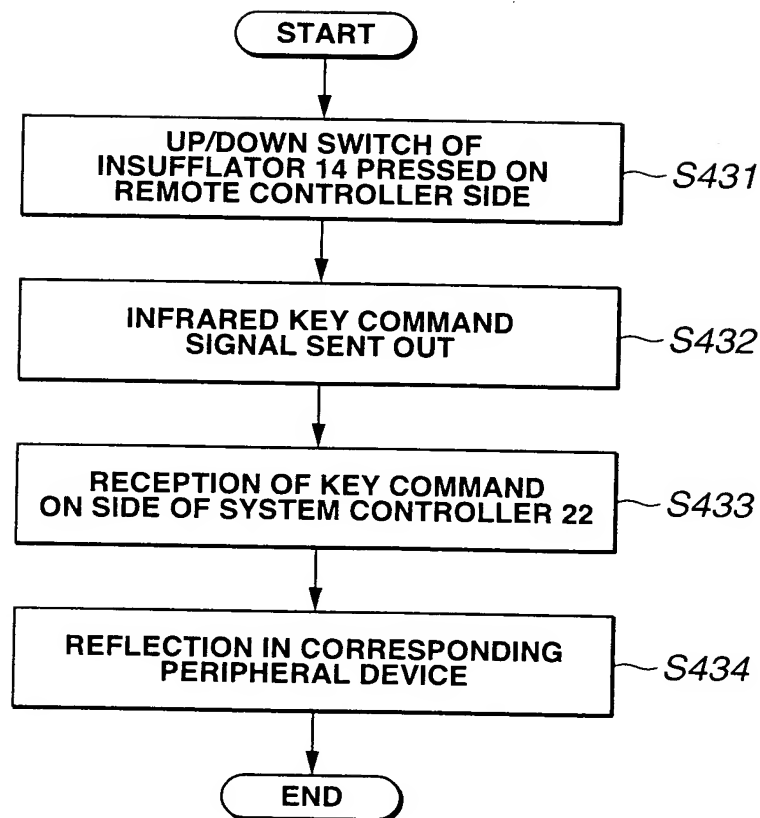


FIG.49

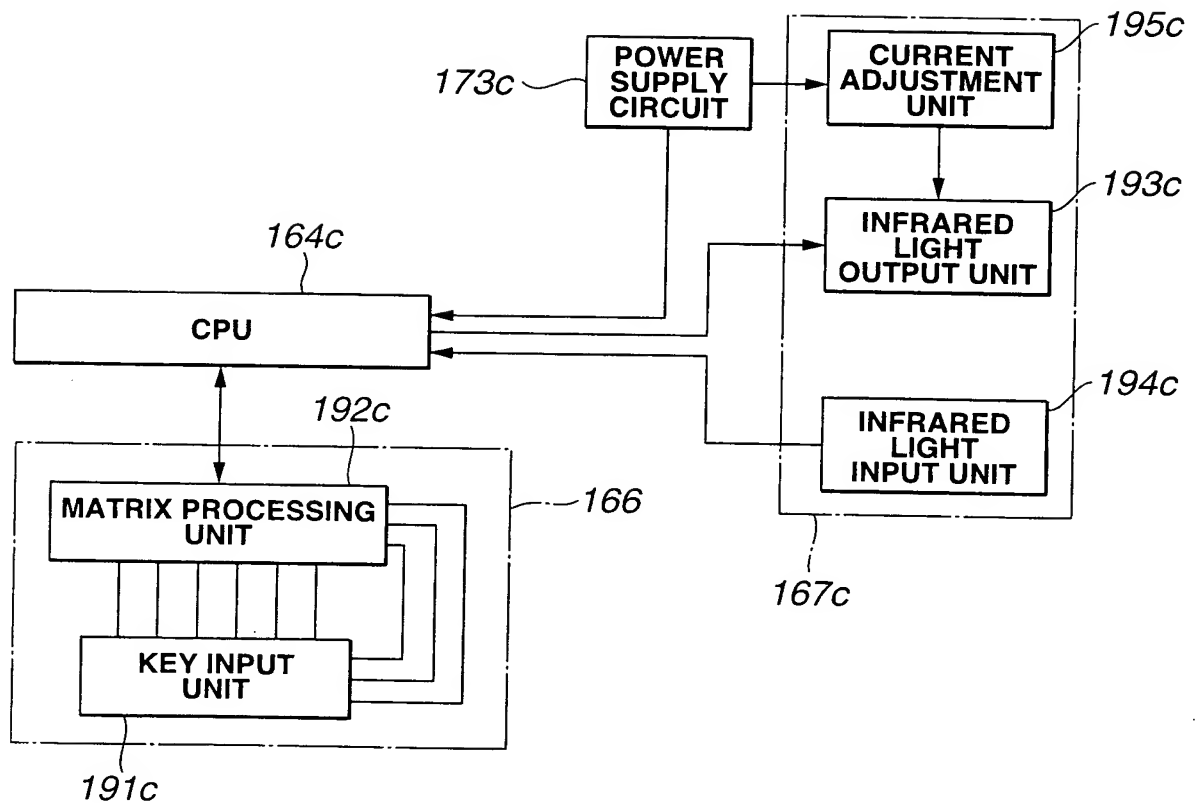


FIG.50

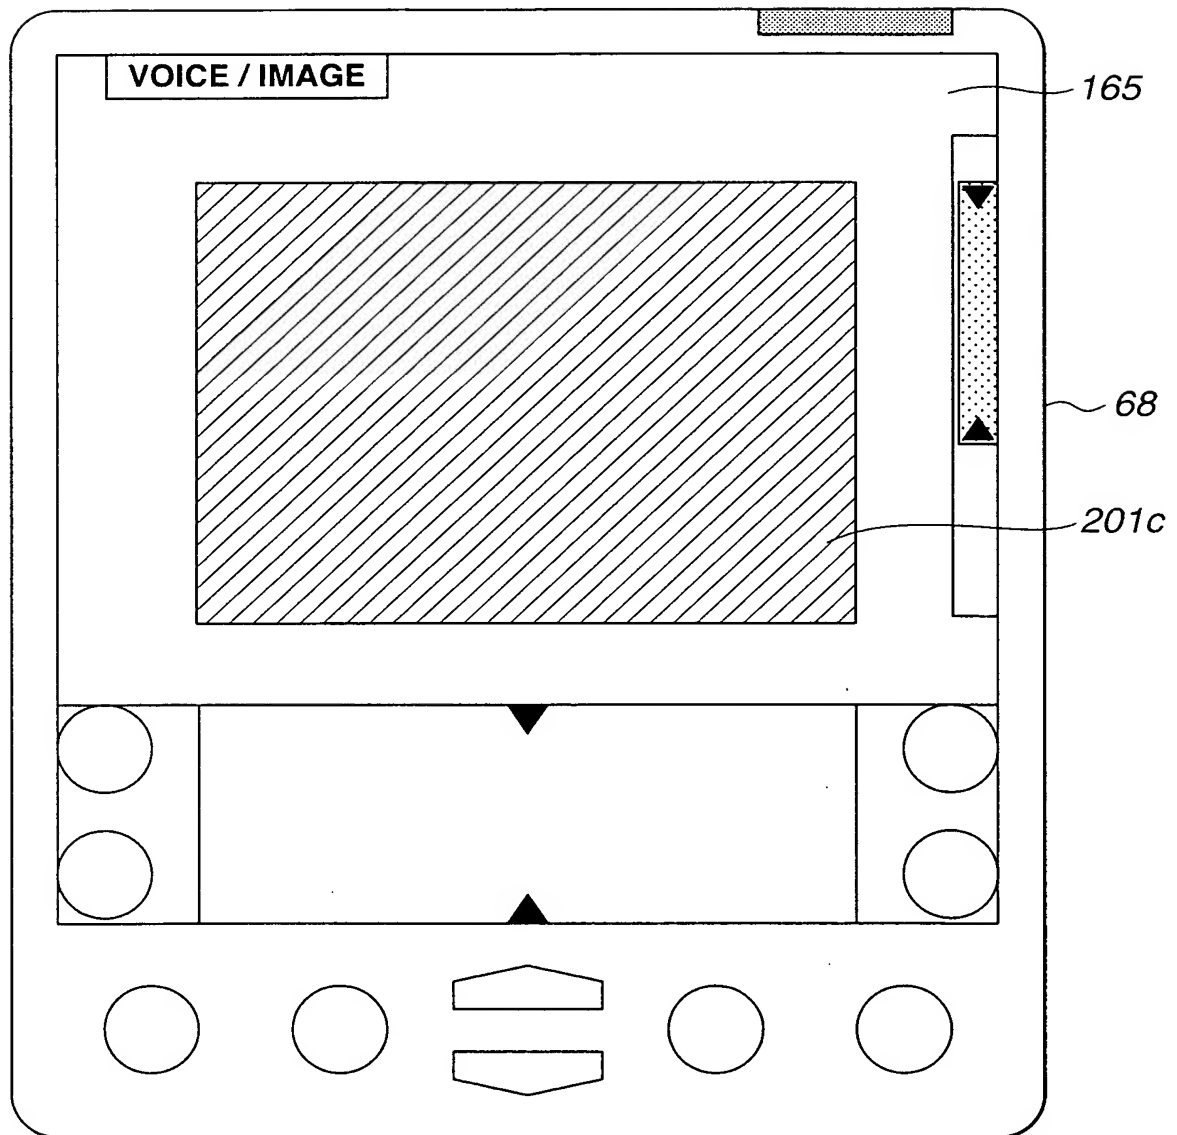


FIG.51

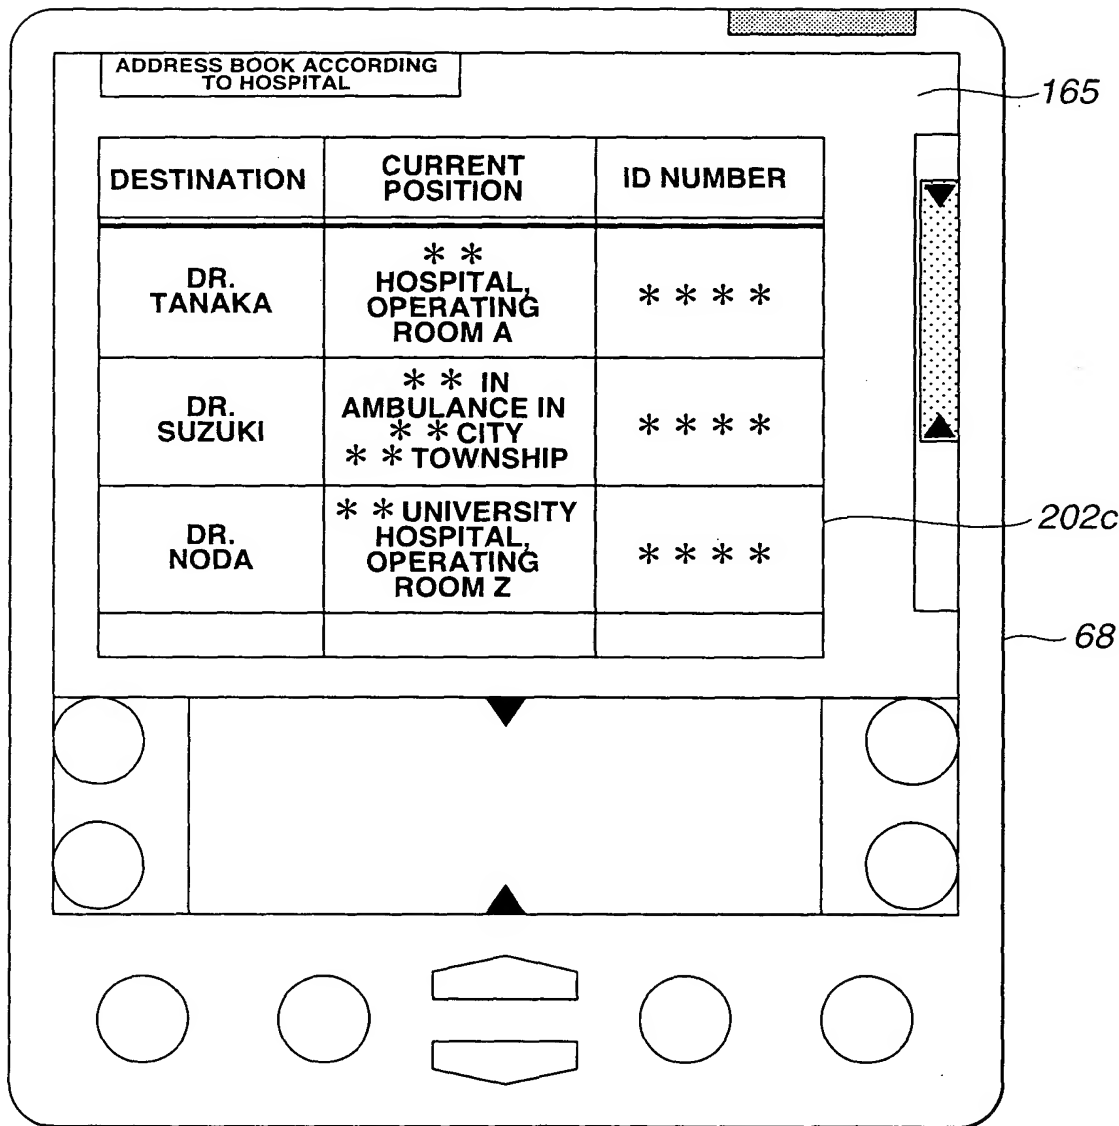


FIG.52

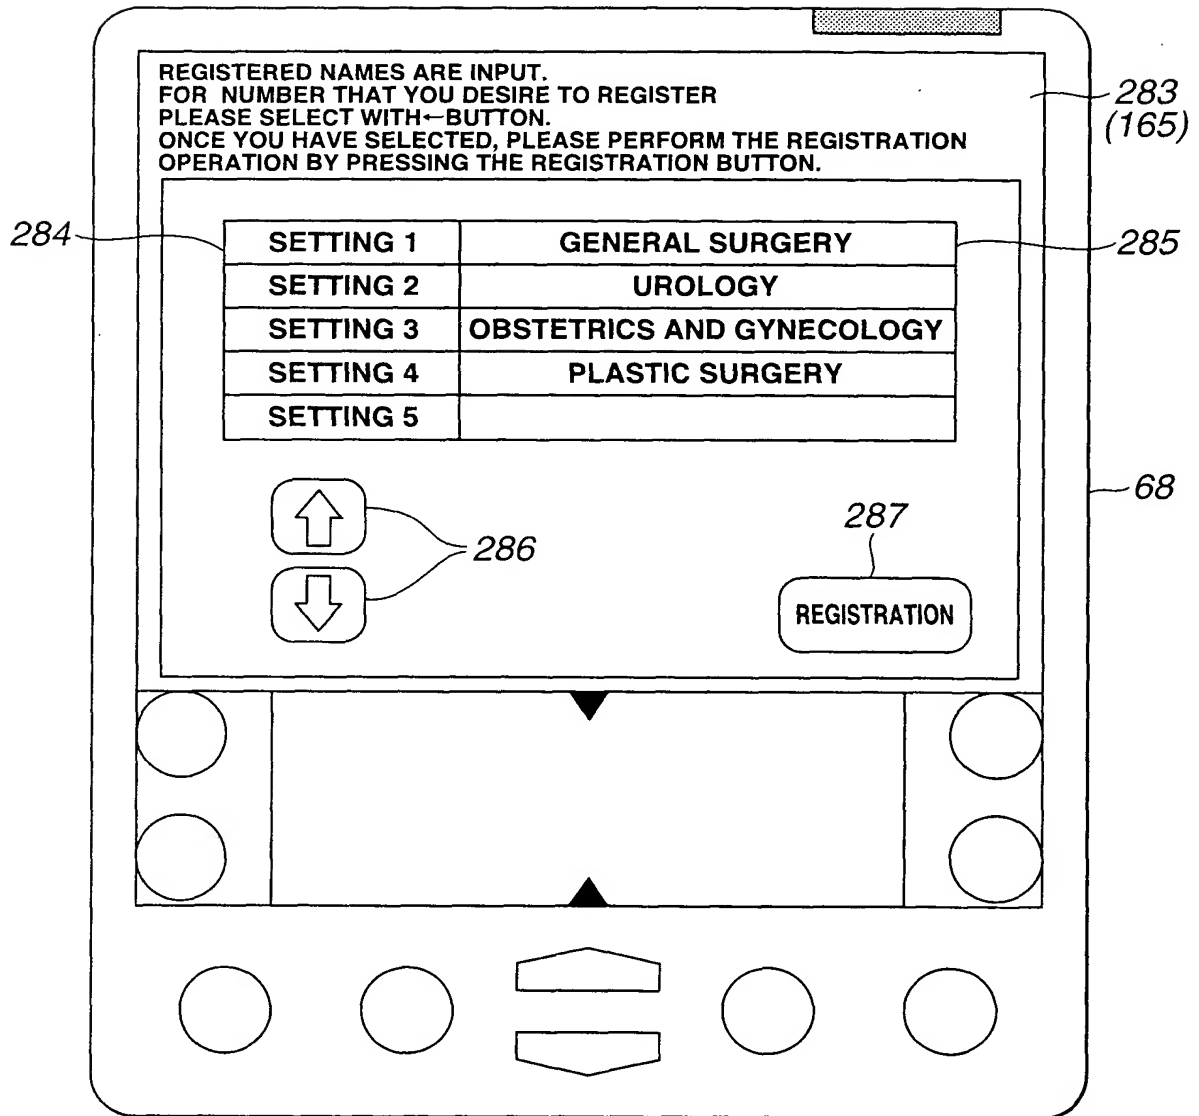


FIG.53

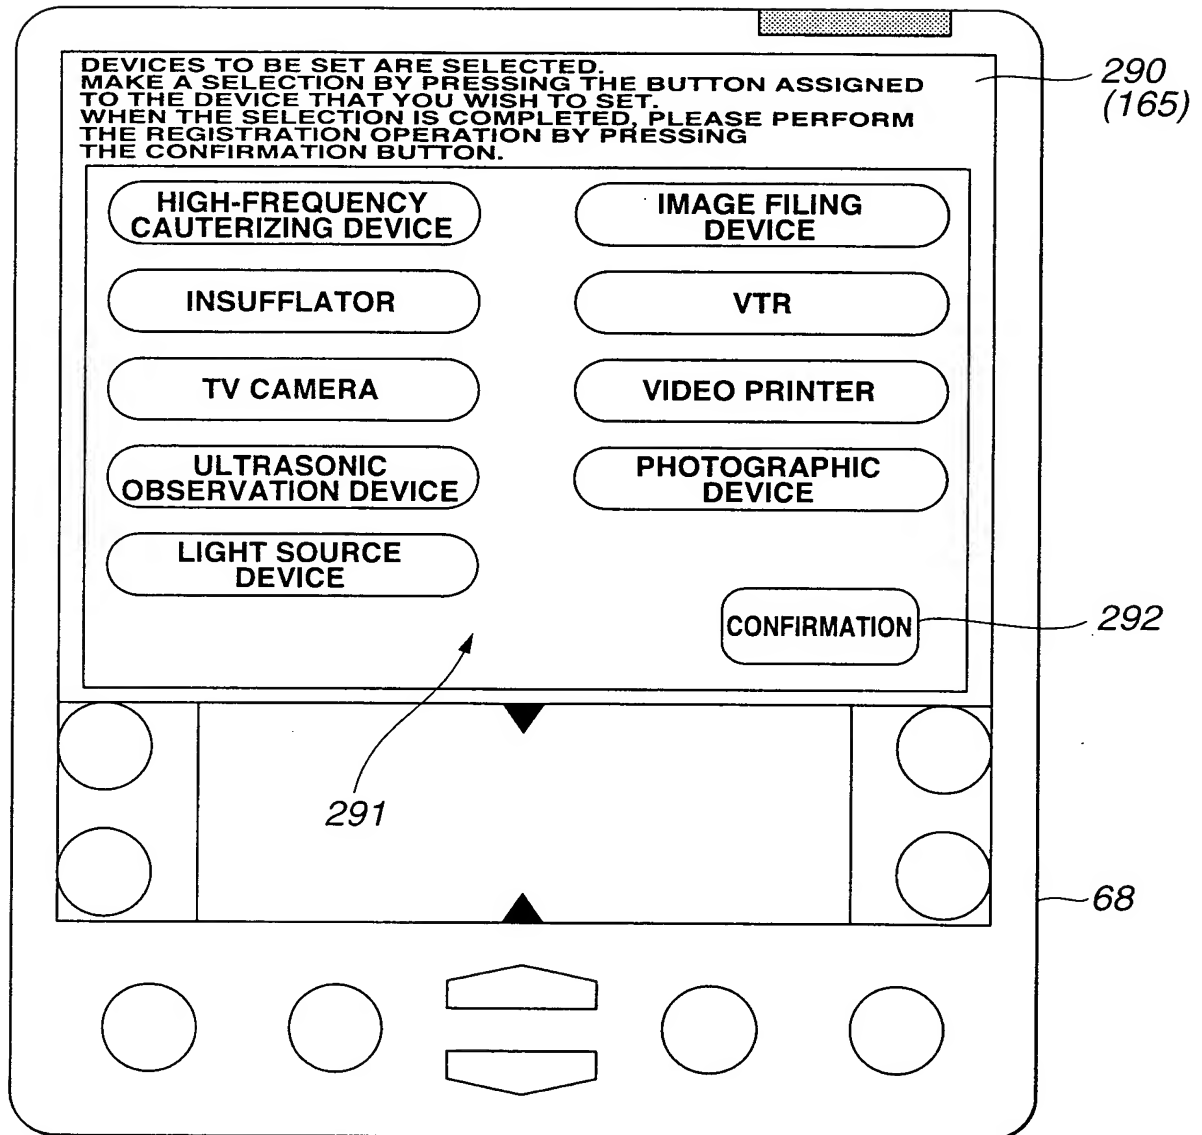


FIG.54

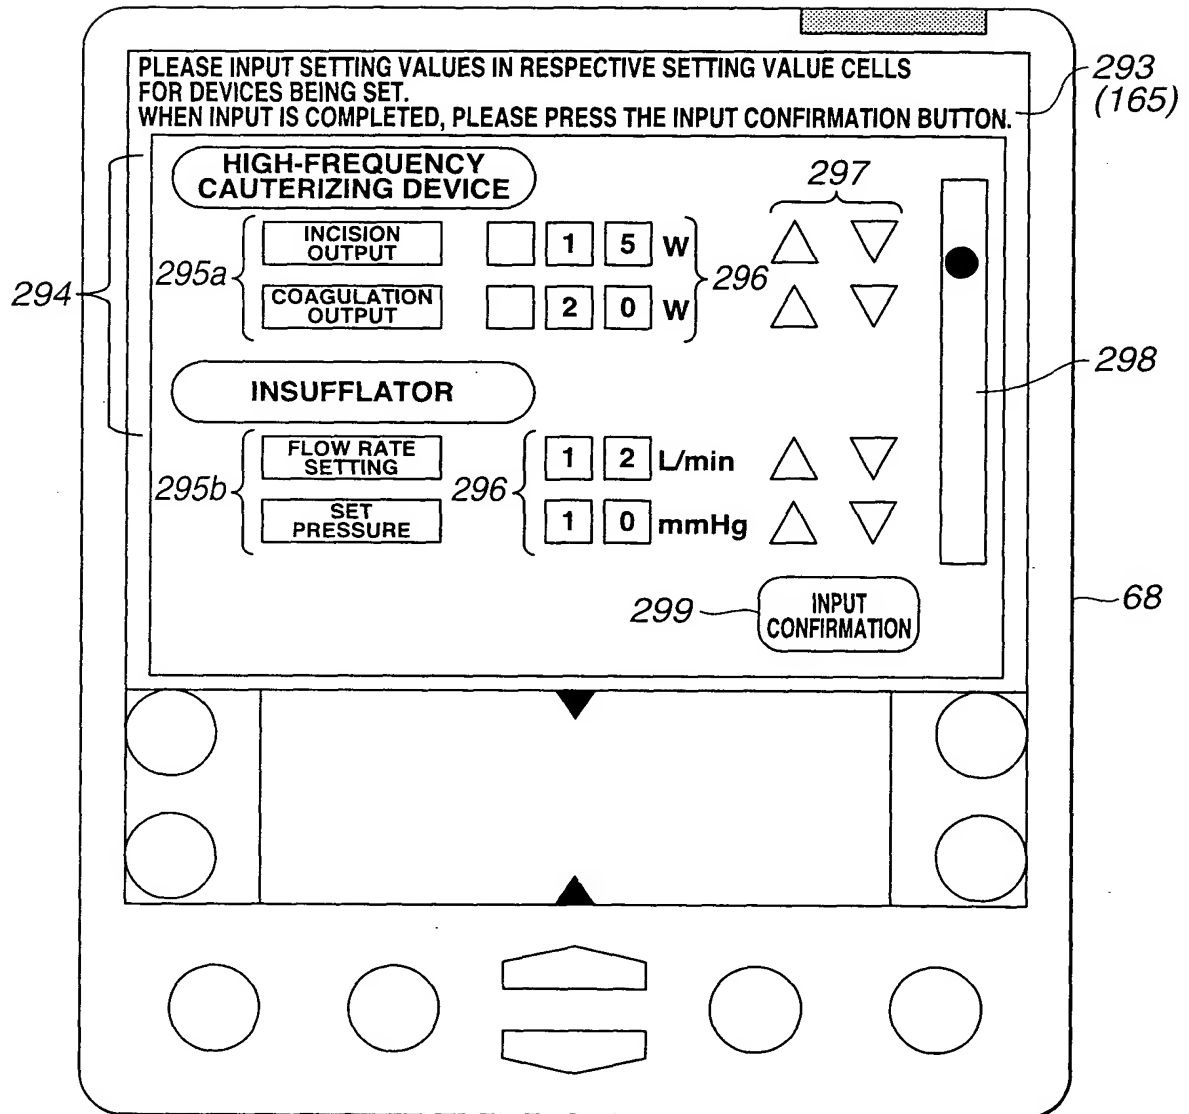


FIG.55

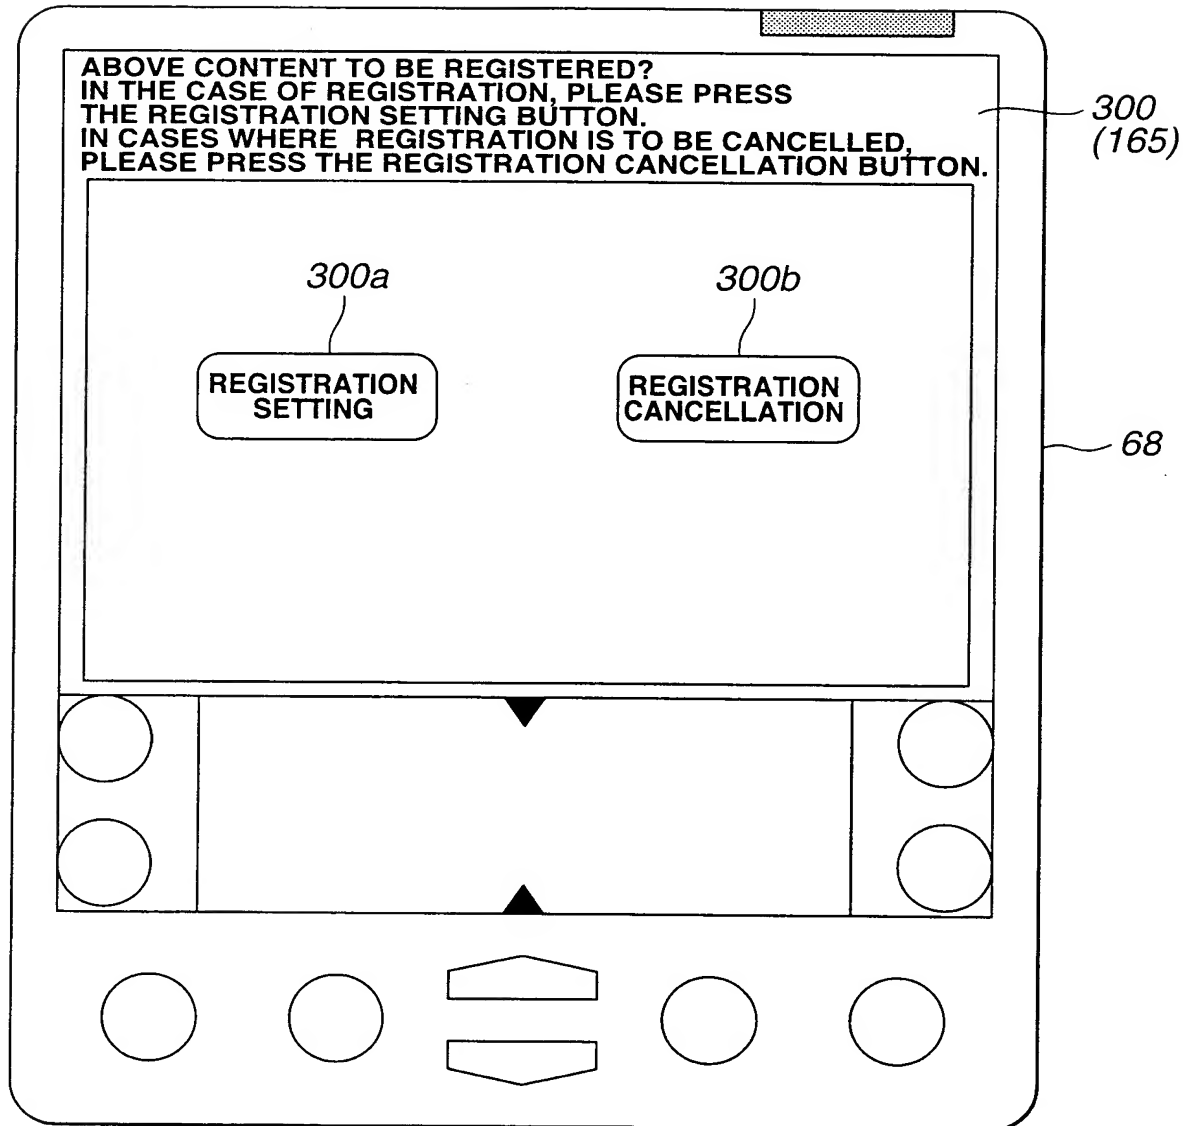


FIG.56

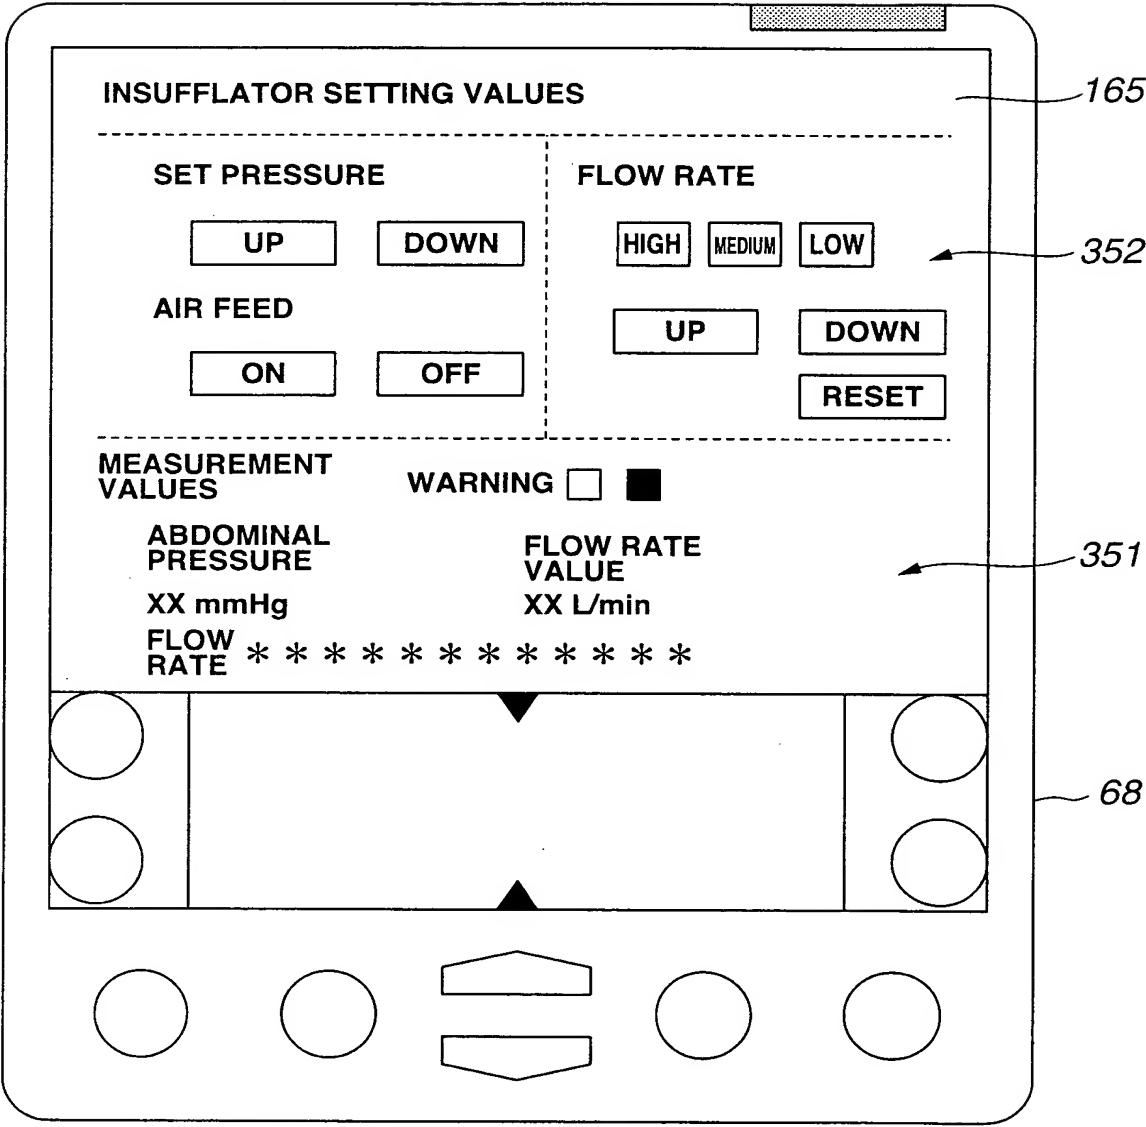


FIG.57

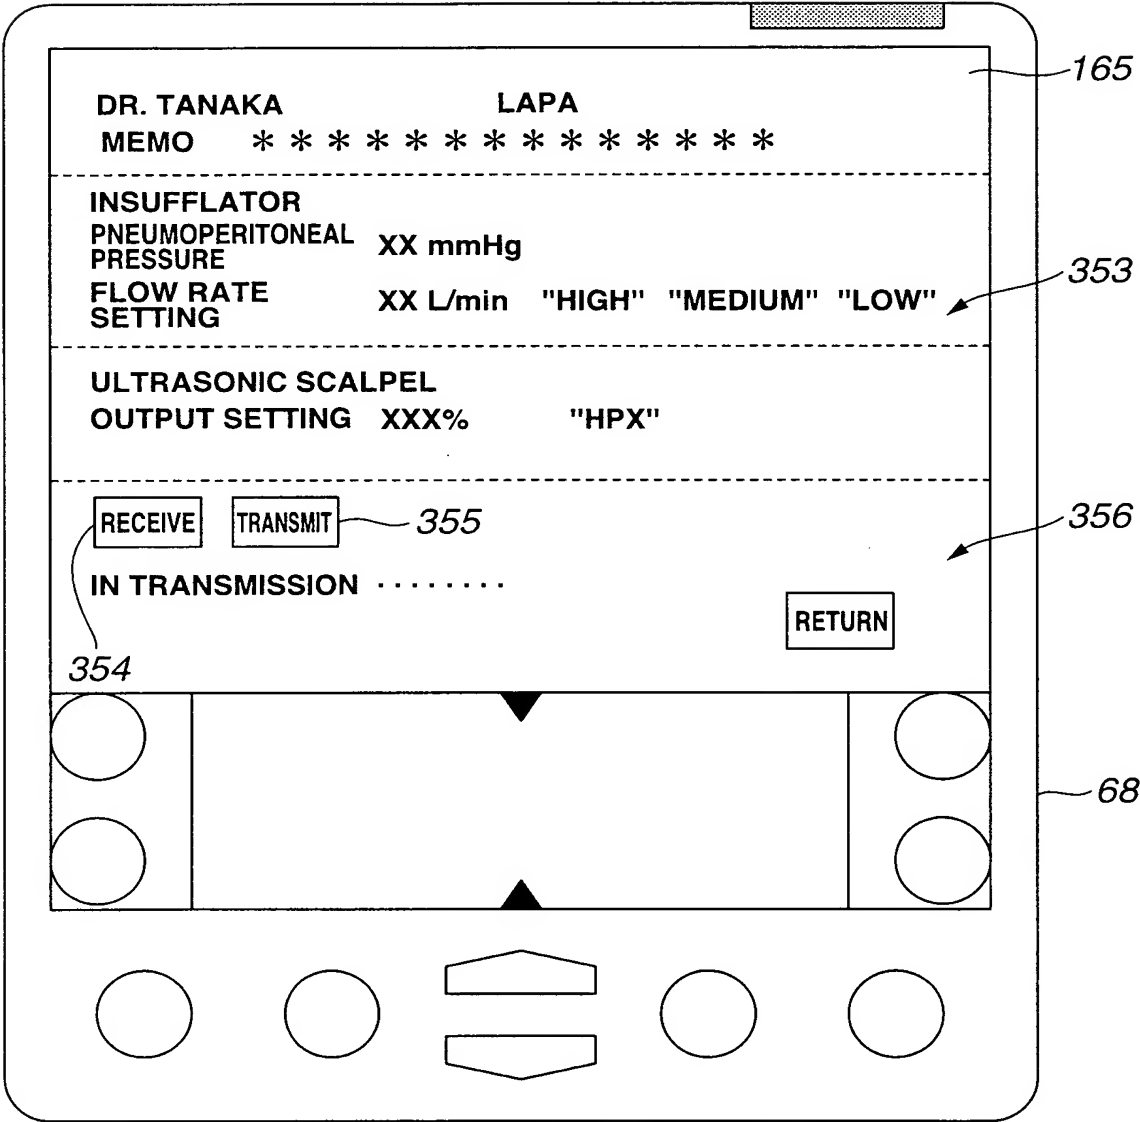


FIG.58


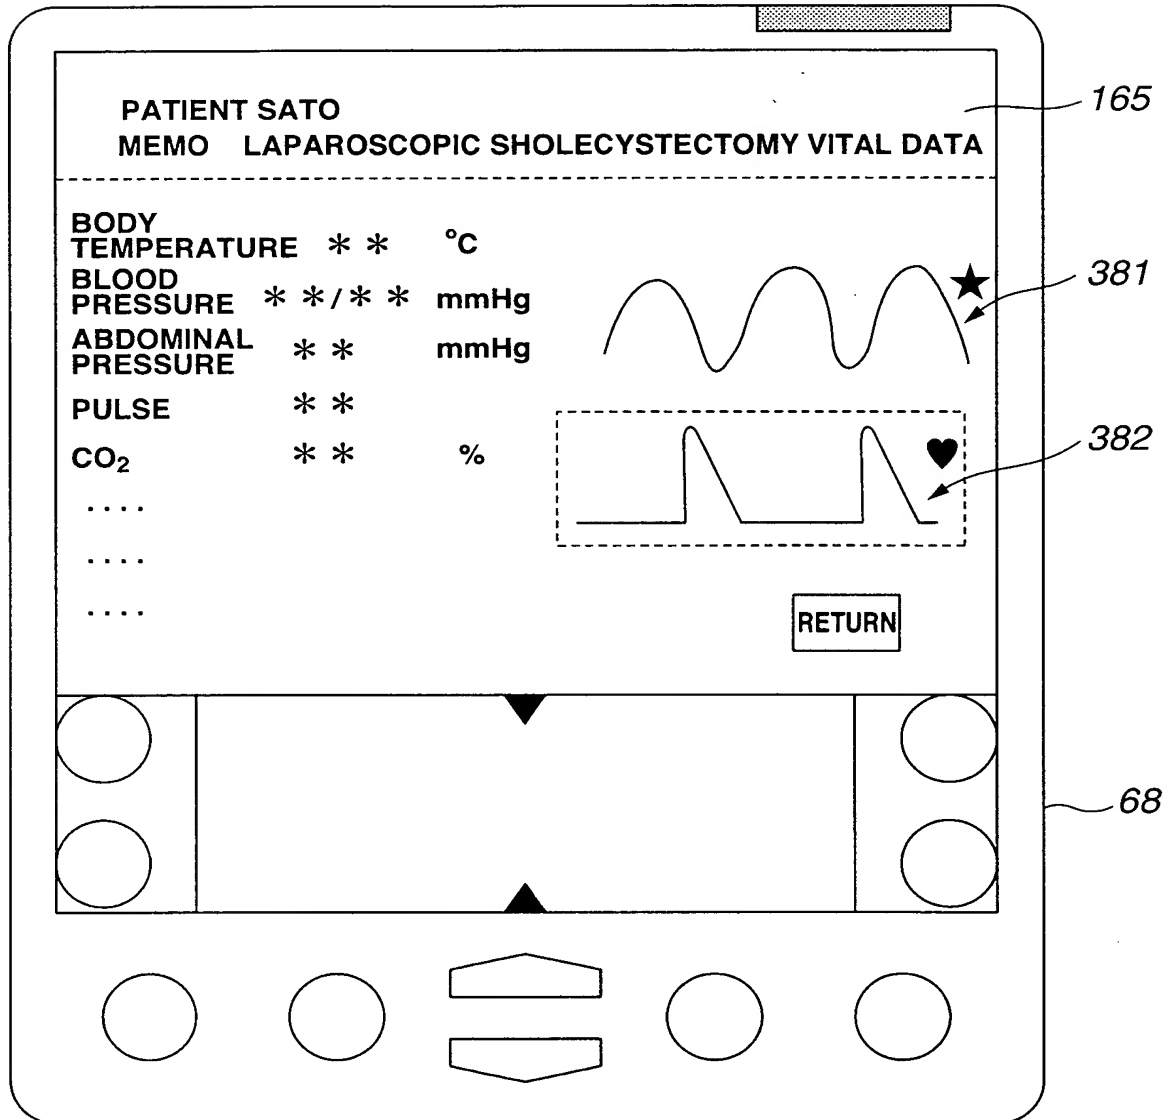


FIG.59

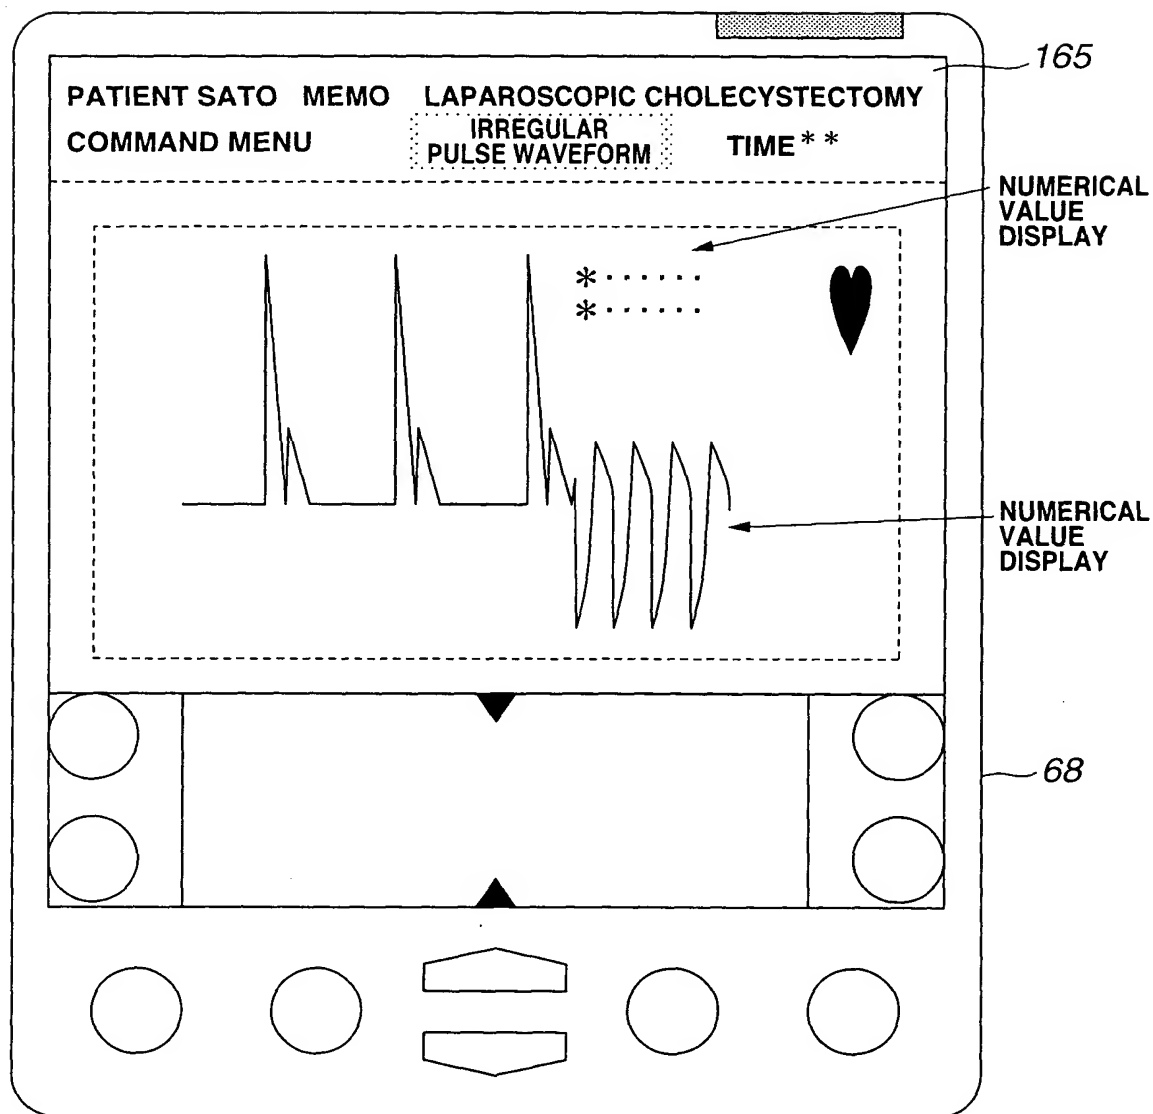

PATIENT SATO MEMO LAPAROSCOPIC CHOLECYSTECTOMY
VATAL DATA

COMMAND MENU ANALYSIS FILTER MATCHING

DATA/TIME	MEASUREMENT VALUE	PATIENT ID	AGE	SEX
* * / * *	* *	* * *	* *	* *
* * / * *	* *	* * *	* *	* *
* * / * *	* *	* * *	* *	* *
* * / * *	* *	* * *	* *	* *
* * / * *	* *	* * *	* *	* *
.....
.....
.....
.....
.....

RETURN

-165

- 68

FIG.61

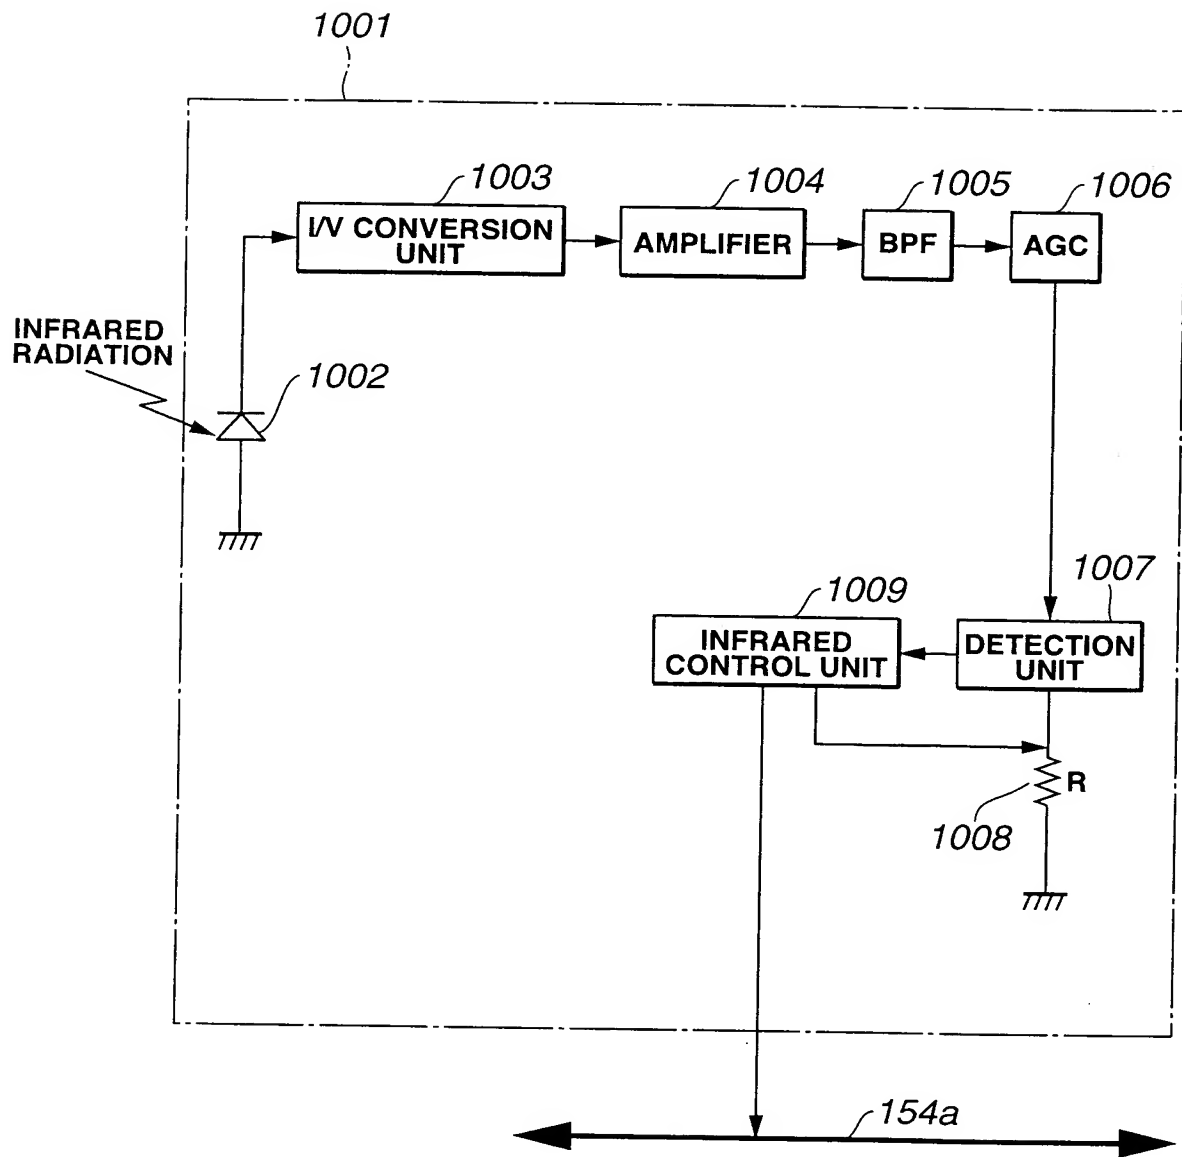


FIG.62

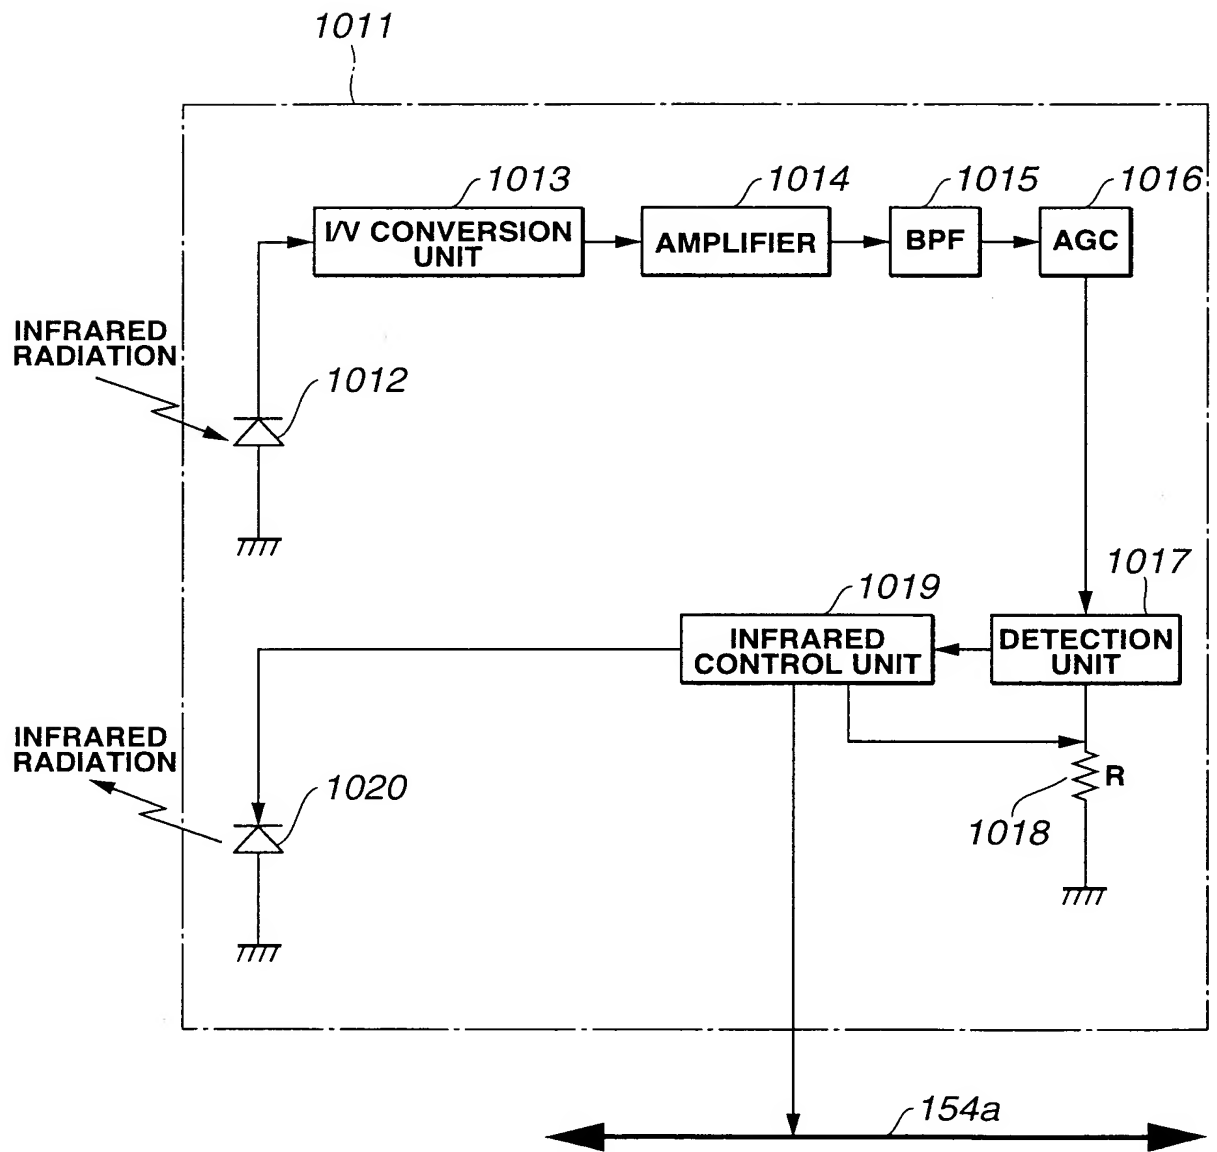


FIG.63

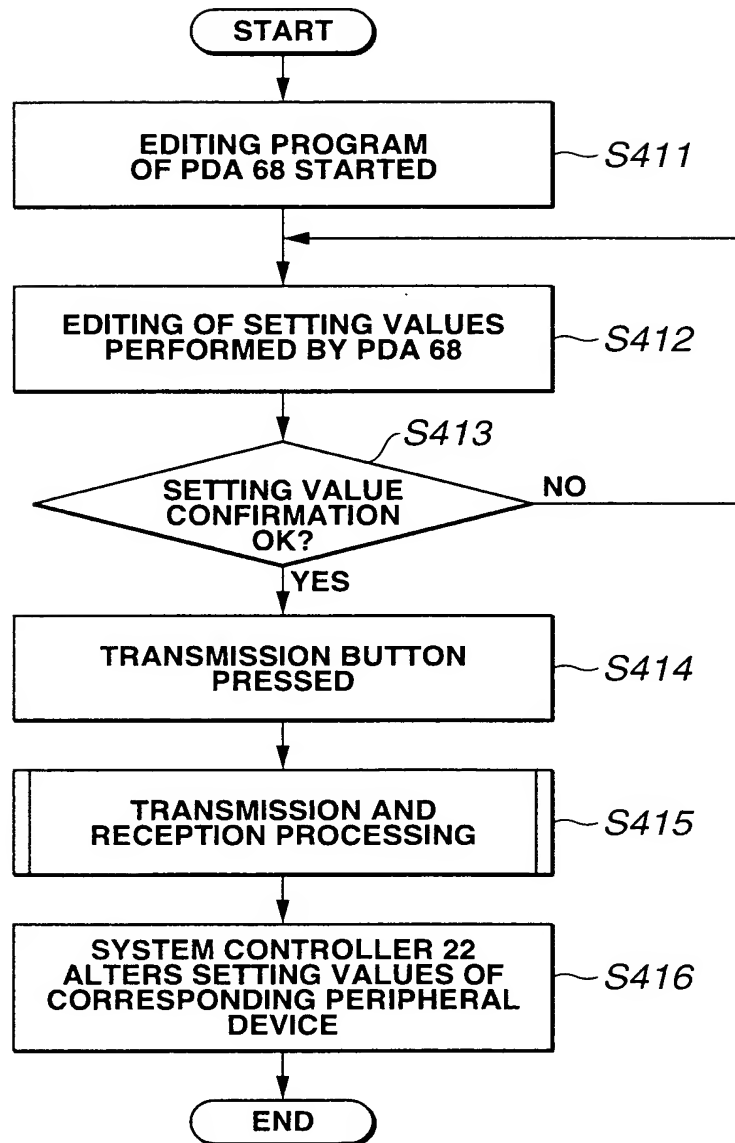


FIG.64

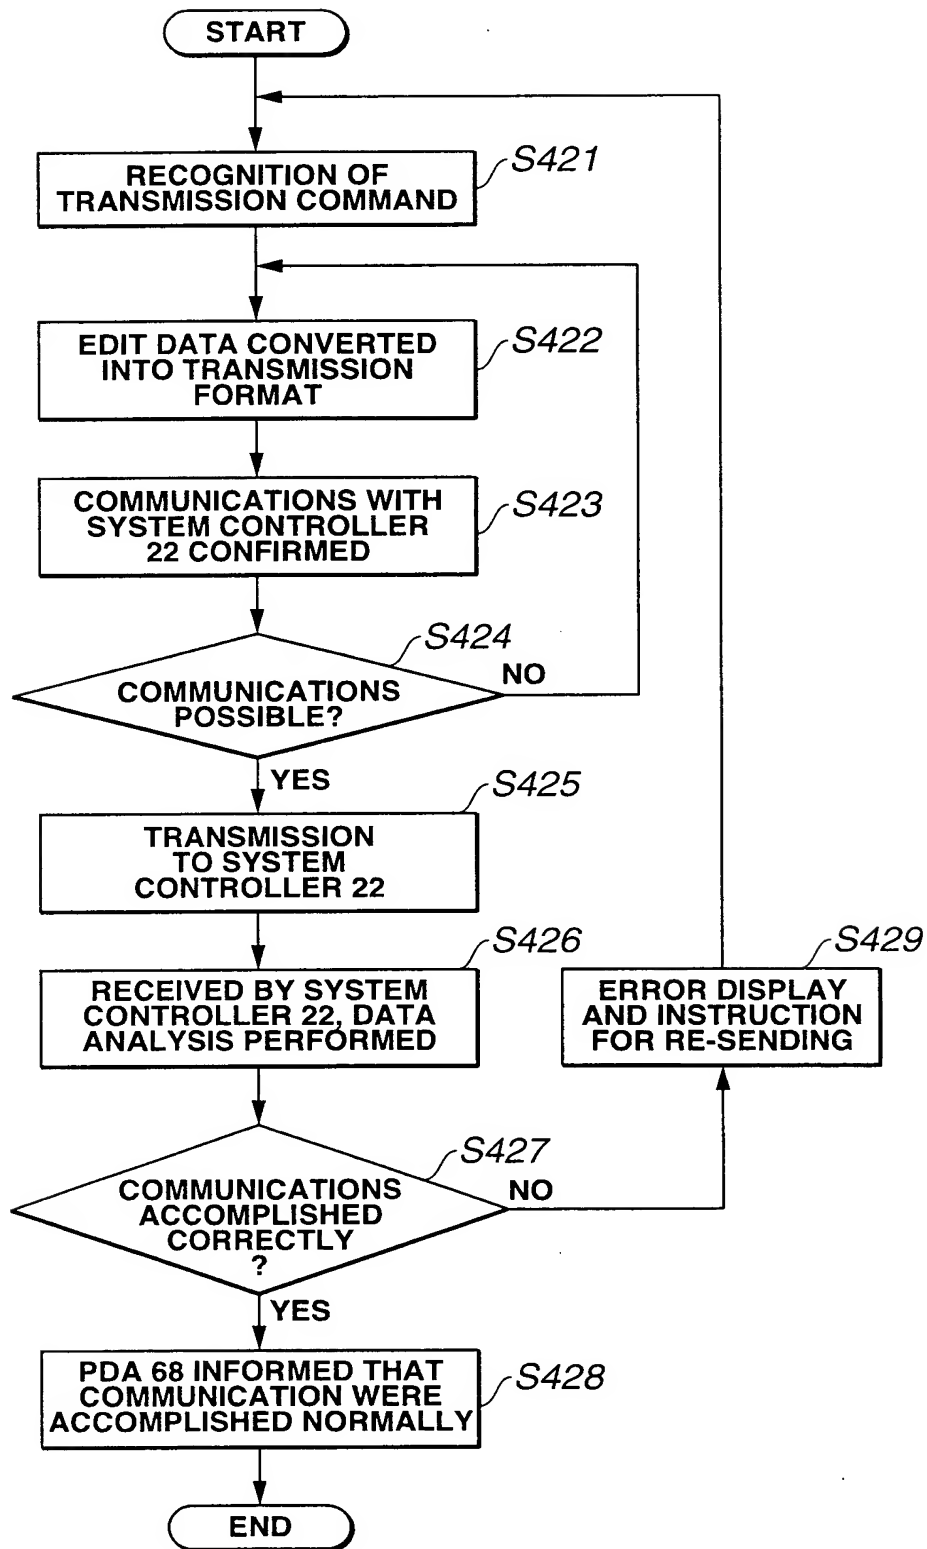


FIG.65

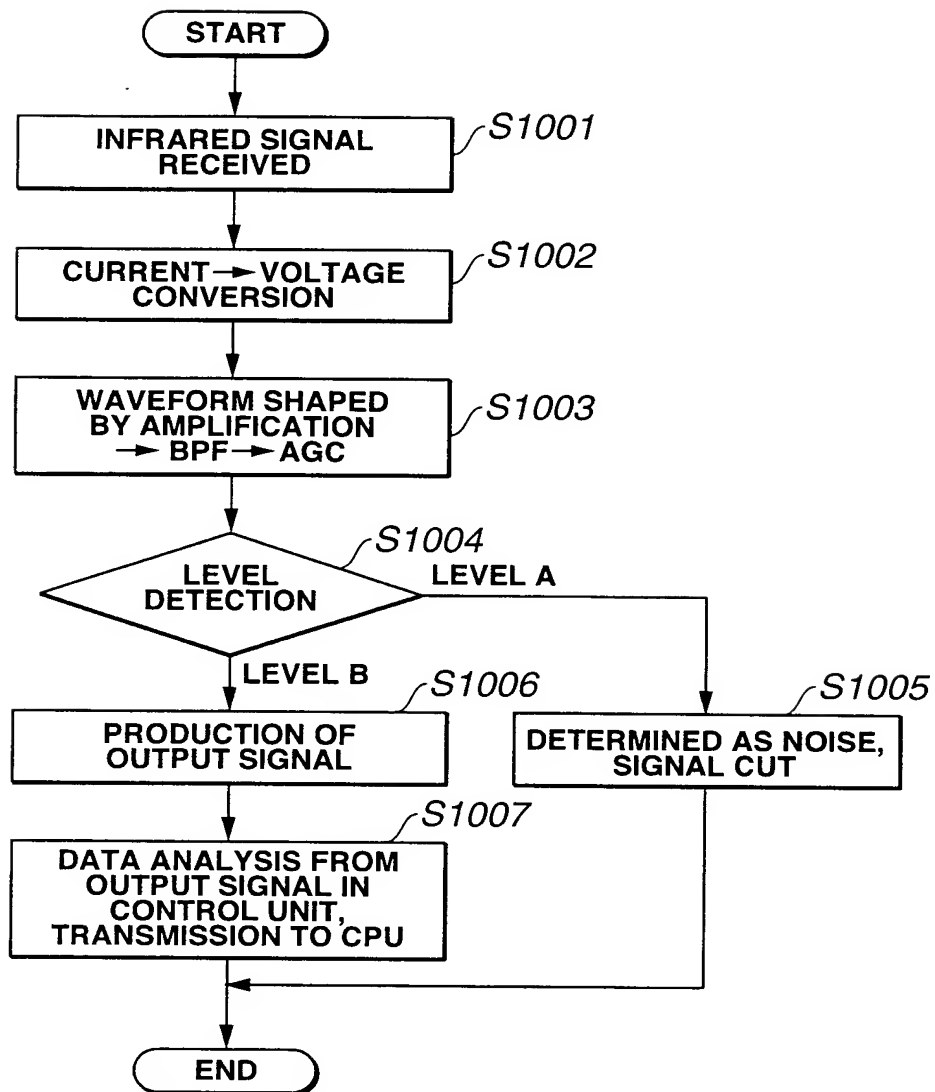


FIG.66

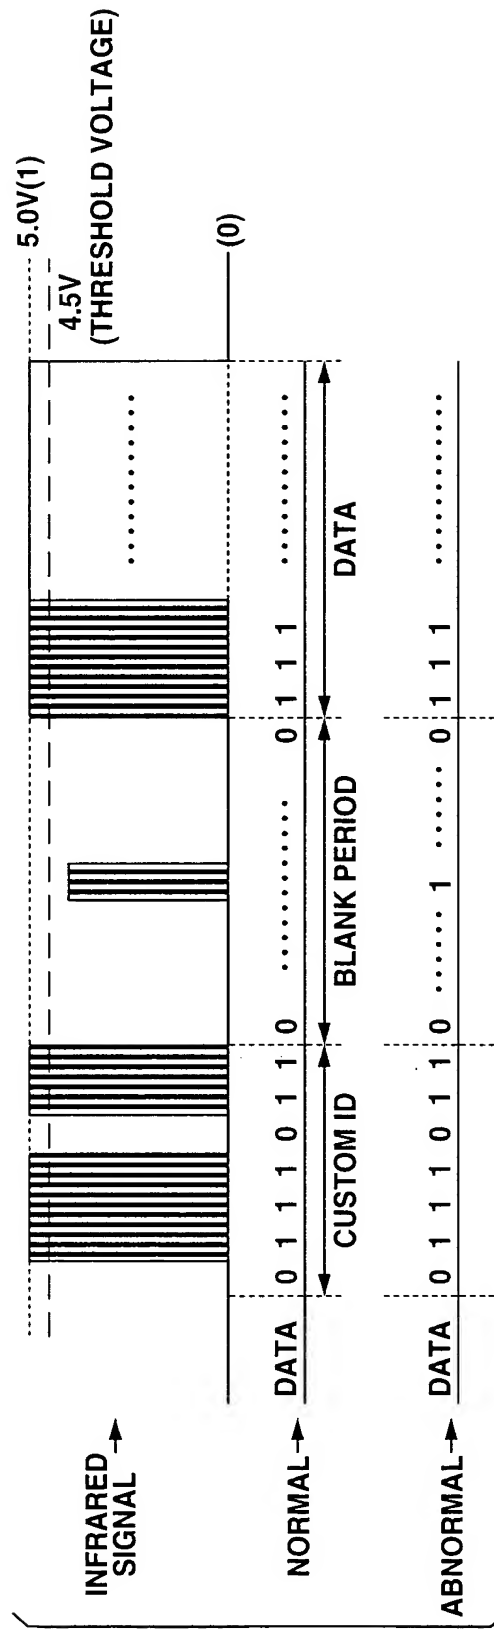


FIG.67

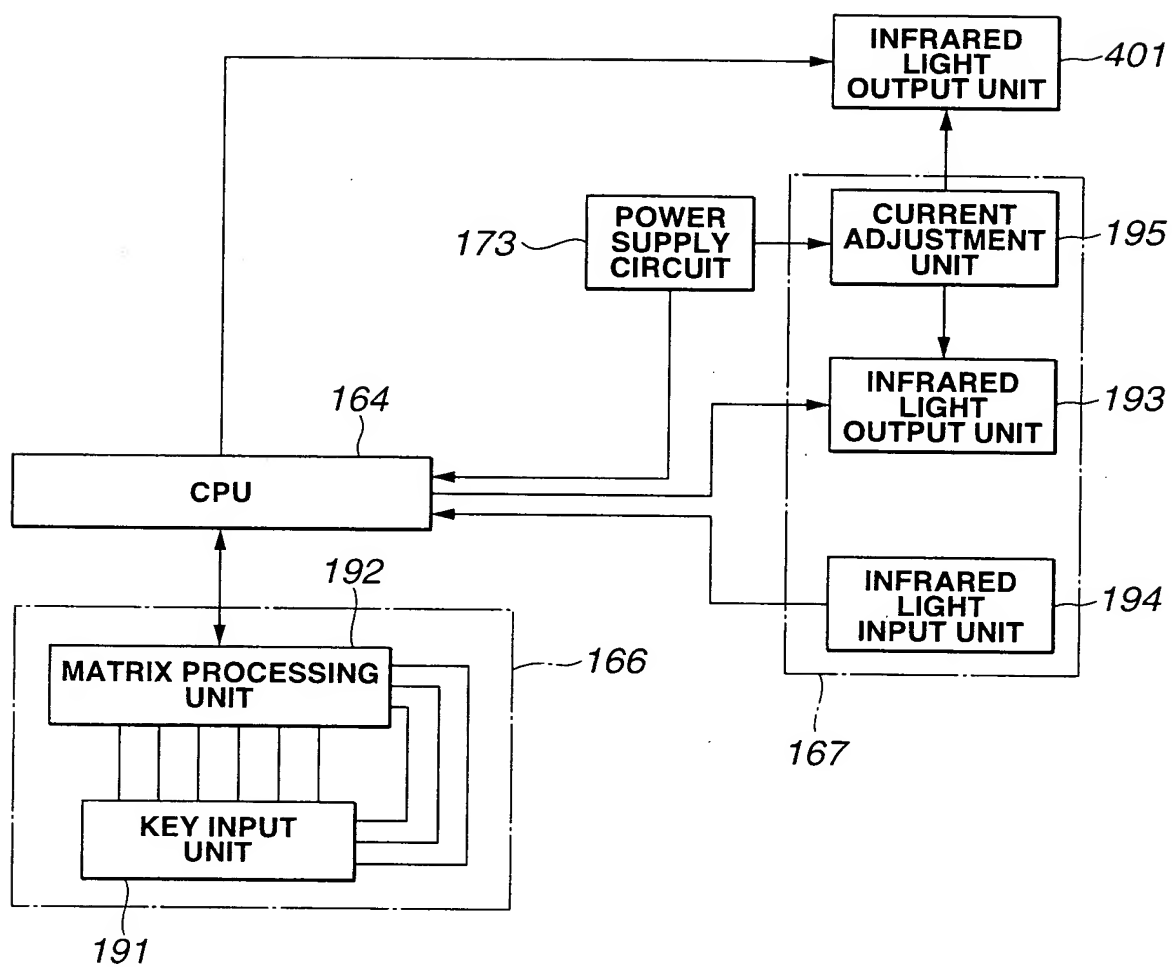


FIG.68

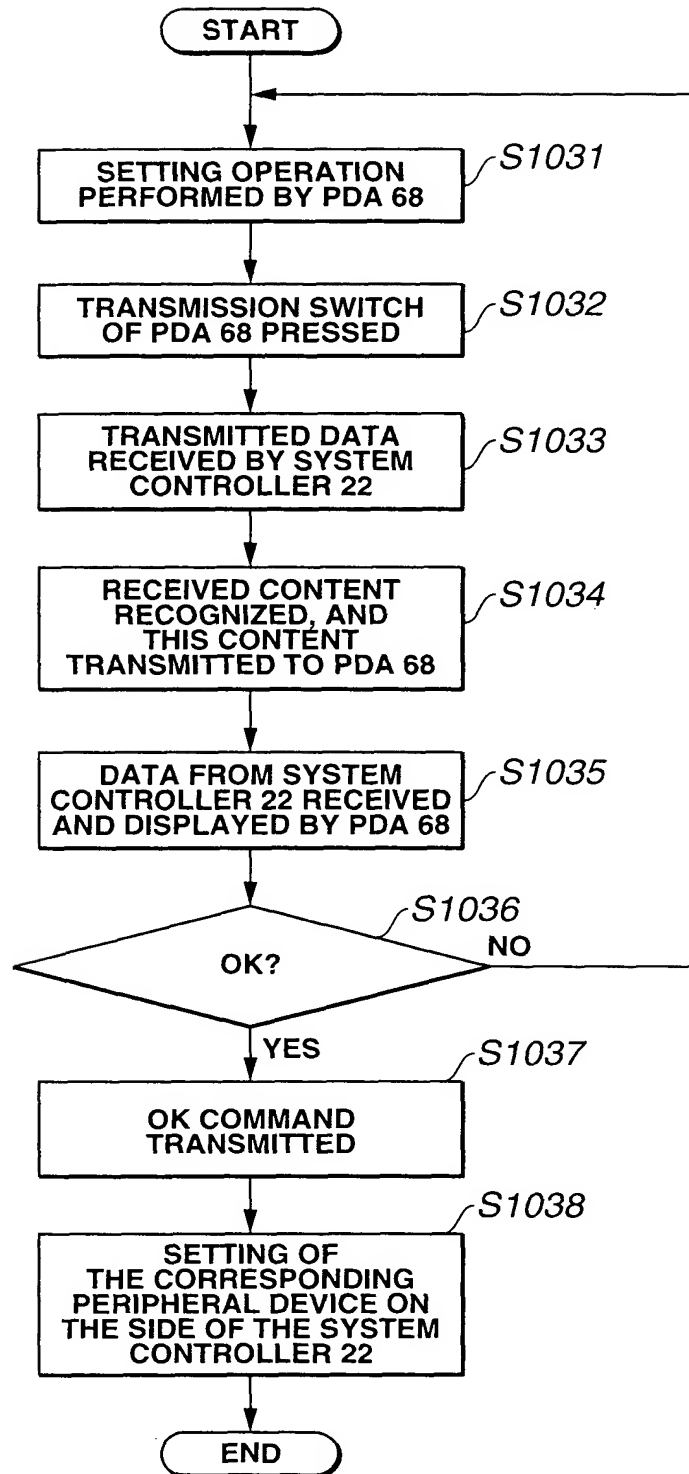


FIG.69

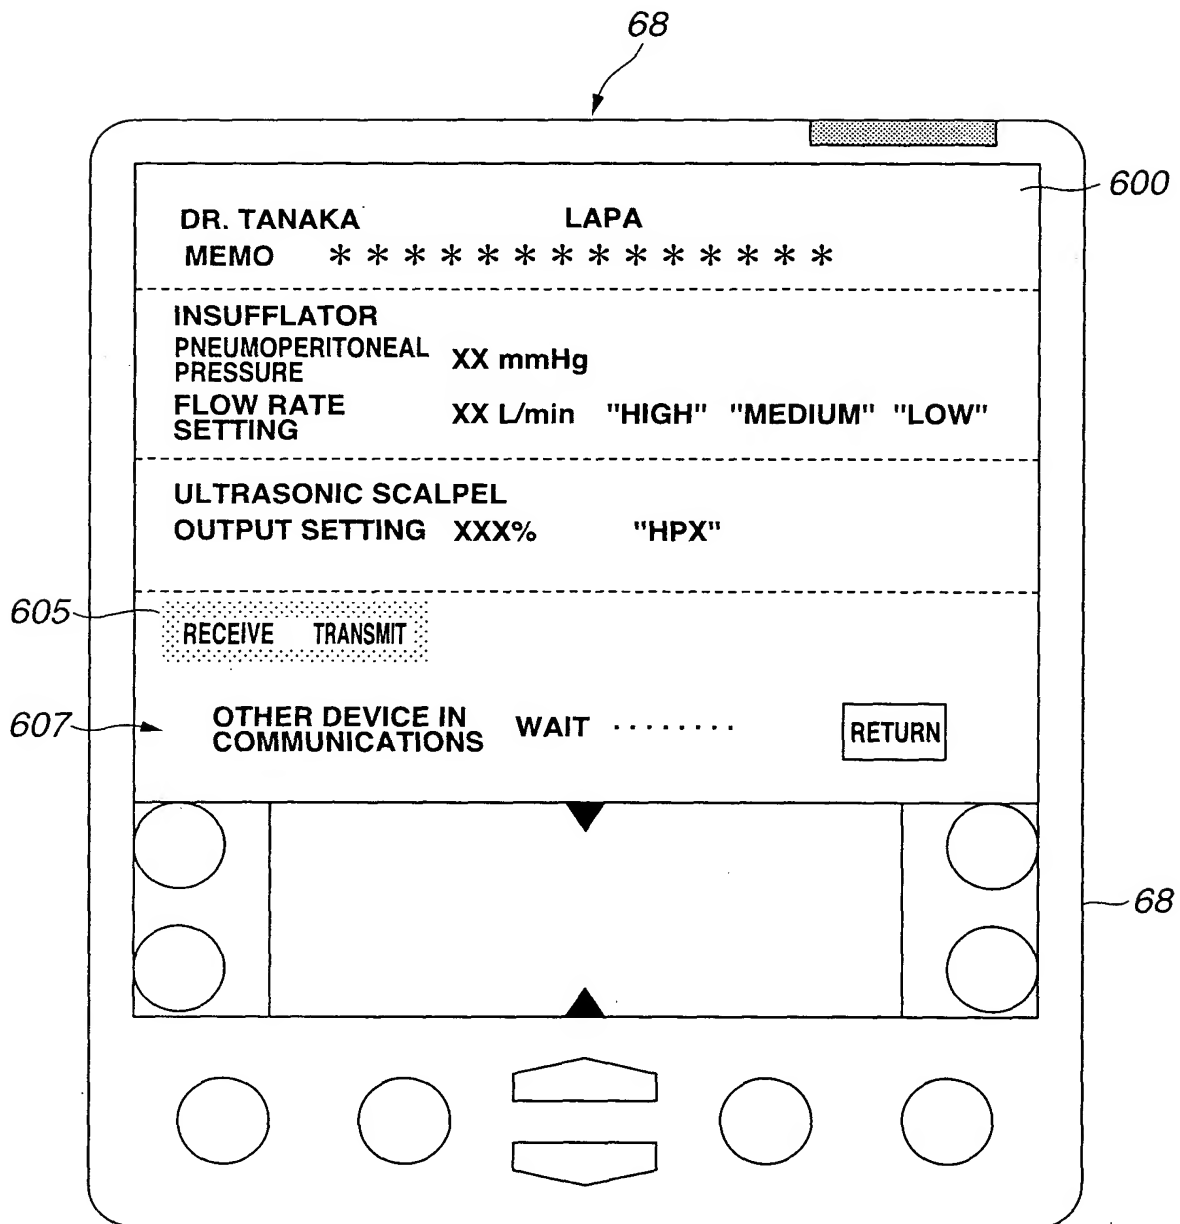


FIG.70

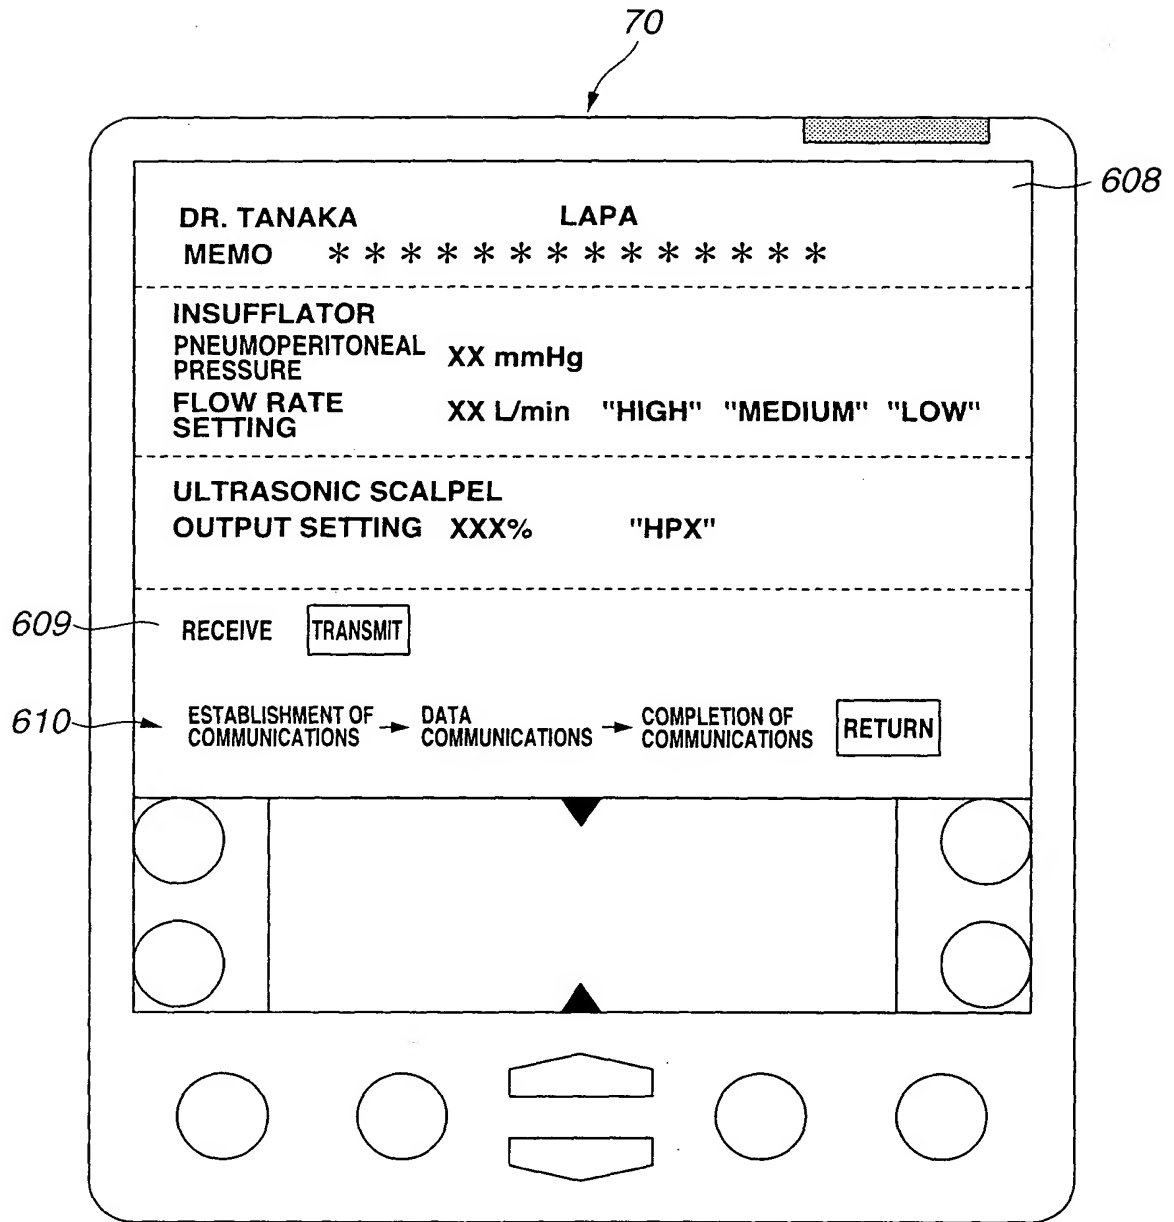


FIG.71

